

Reliability Report

June 2023

IMPLANTABLE COCHLEAR STIMULATORS
AND SOUND PROCESSORS

POWERFUL CONNECTIONS



START HERE

An Update from the President of Advanced Bionics	4
Implantable Cochlear Stimulators	6
HiRes Ultra 3D (V2) cochlear implant	8
HiRes Ultra (V2) cochlear implant	10
HiRes Ultra 3D (V1) cochlear implant	12
HiRes Ultra (V1) cochlear implant	14
HiRes 90K Advantage cochlear implant	16
HiRes 90K cochlear implant	18
CII Bionic Ear cochlear implant	26
Clarion 1.2 cochlear implant	28
Clarion 1.0 cochlear implant	30
Sound Processor Stimulators	32
Naída CI M and Sky CI M sound processors	33
Naída CI Q90 sound processor	34
Chorus sound processor	34
Neptune sound processor	35
Appendix	36



A MESSAGE FROM THE PRESIDENT OF ADVANCED BIONICS

Throughout 2023, Advanced Bionics is celebrating three decades of connections with hearing healthcare professionals to supply quality innovative technologies which empower our recipients to expand their own strong connections. We are proud to present our latest cochlear implant and sound processor reliability data, demonstrating our commitment to delivering best-in-class reliability and transparent quality reporting which exceeds global standards.

Advanced Bionics' goal is to meet the needs of our recipients by delivering products created through stringent manufacturing and testing processes. Our dedication to delivering high quality products has given rise to the HiRes Ultra 3D v2 with industry leading reliability according to international reporting methodologies.

AB's connections with the world-wide cochlear implant community have been built based on transparent communication. When you work with the people and products of Advanced Bionics, you can feel confident that you are collaborating with an organization dedicated to meeting or exceeding reporting methodologies recommend by both the International Organization for Standardization^{1,2} and ANSI/AAMI CI 86.³

As we mark AB's 30-year anniversary creating powerful connections, we look forward to continuing to deliver reliable and innovative hearing enabling products, furthering trust through transparent communication, and helping to empower those with hearing loss to experience powerful connections.



Victoria E. Carr-Brendel, Ph.D.
PRESIDENT, ADVANCED BIONICS

1. ISO 5841-2 (2014) Implants for Surgery – Cardiac Pacemakers. International Organization for Standardization (ISO), Geneva, Switzerland.
2. European Consensus Statement on Cochlear Implant Failures and Explanations. (2005) *Otology and Neurology*, 26(6): 1097-1099.
3. ANSI/AAMI CI86. Cochlear Implant Systems: Requirements for Safety, Functional Verification, Labeling and Reliability Reporting. (2017). Arlington, VA: American National Standards Institute.



INTERPRETING TABLES AND GRAPHS

IMPLANTABLE COCHLEAR STIMULATORS


Number of registered HiRes Ultra 3D V2 implants

As of April 3, 2023.
Date of first commercial introduction: 2019.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	14408	5025	19433 ^b
ANSI/AAMI CI86	15313 ^c	4120	19433

Number of registered users is detailed for adults, children (defined as less than 18 years at implantation by ISO 5841, and less than 10 years at implantation by CI86), and a combination of all ages in accordance with reporting methodologies.

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
- b. The combined number also includes any registered users for whom we do not have date of birth information.
- c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

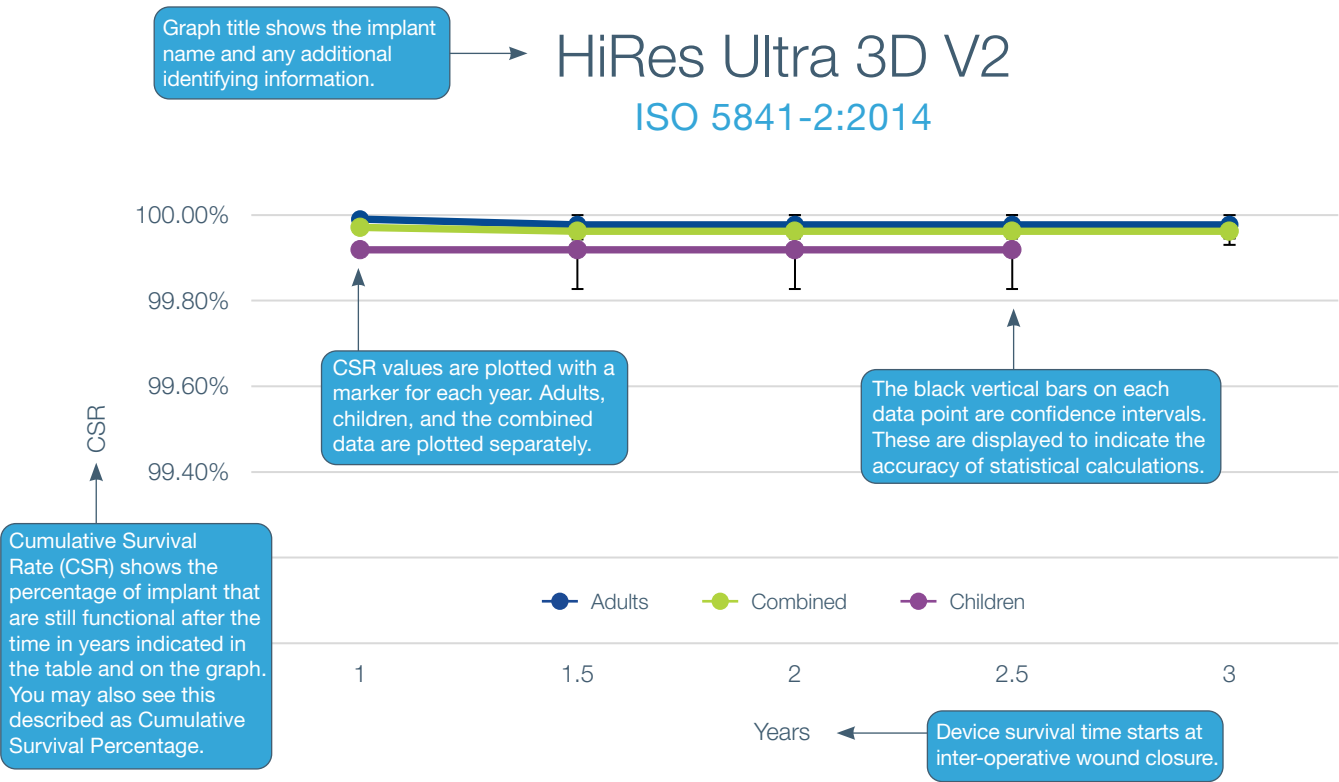

CUMULATIVE SURVIVAL RATE


Years in use	1	1.5	2	2.5	3
ADULTS	99.99%	99.98%	99.98%	99.98%	99.98%
COMBINED	99.97%	99.96%	99.96%	99.96%	99.96%
CHILDREN	99.92%	99.92%	99.92%	99.92%	N/A*

Detailed CSR percentages are shown for each year in the table. Results are shown as: adult, children and combined total.

*Sample size is not large enough for reporting

Graph title shows the implant name and any additional identifying information.

HiRes Ultra 3D V2 ANSI/AAMI CI86 STANDARD

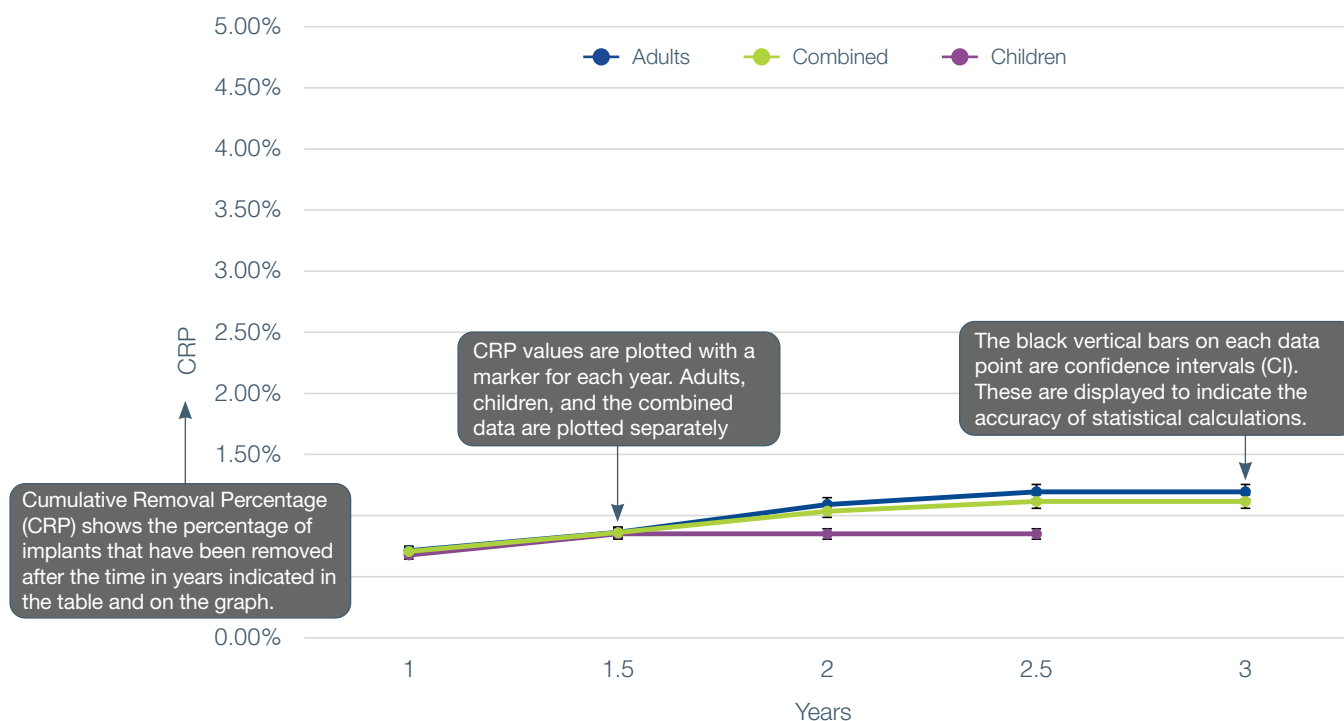

The ANSI/AAMI CI86 Standard requires that all removed devices are classified into three categories based on the rationale for explantation: device failure, medical reason, or inconclusive.

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.68%	0.03%	0.00%	0.71%	0.84%	0.58%
1.5	0.82%	0.04%	0.00%	0.86%	1.01%	0.71%
2	1.00%	0.04%	0.00%	1.04%	1.22%	0.86%
2.5	1.08%	0.04%	0.00%	1.12%	1.32%	0.91%
3	1.08%	0.04%	0.00%	1.12%	1.32%	0.91%

Throughout this report, we will present the data and graphs to represent the conditions for: analysis by category for adults and children; removal rates by analysis category for adults and children, and all analysis categories for adults and children combined.

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

CURRENT-GENERATION IMPLANT DATA

HIRES ULTRA 3D V2

The HiRes™ Ultra 3D (V2) cochlear implant is an update to the previous HiRes Ultra 3D (V1) device. Based off the standard HiRes Ultra platform but featuring an innovative multi-magnet assembly, the HiRes Ultra 3D V2 implant allows the use of clinical MRI at 1.5T and 3T without the need for magnet removal or head-bandaging. Due to the low torque, the recipient can be expected to have a hassle free and pain free experience.

The HiRes Ultra 3D (V2) device has a Cumulative Survival Rate (CSR) of 99.96%.



Number of registered HiRes Ultra 3D V2 implants

As of April 3, 2023.

Date of first commercial introduction: 2019.^a


STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	14408	5025	19433 ^b
ANSI/AAMI CI86	15313 ^c	4120	19433

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.

b. The combined number also includes any registered users for whom we do not have date of birth information.

c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

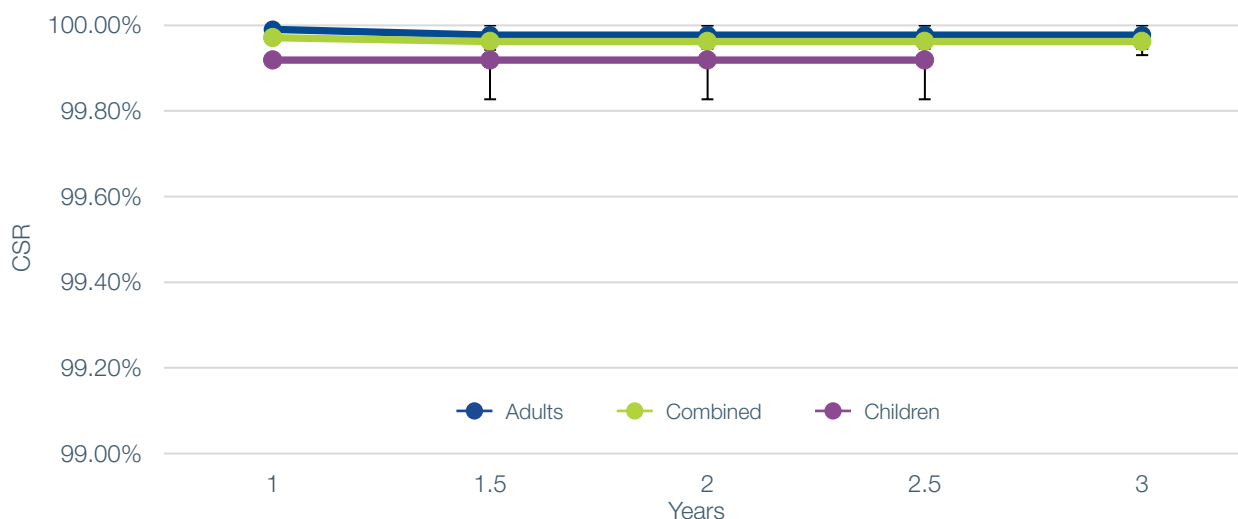


CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3
ADULTS	99.99%	99.98%	99.98%	99.98%	99.98%
COMBINED	99.97%	99.96%	99.96%	99.96%	99.96%
CHILDREN	99.92%	99.92%	99.92%	99.92%	N/A*


*Sample size is not large enough for reporting

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

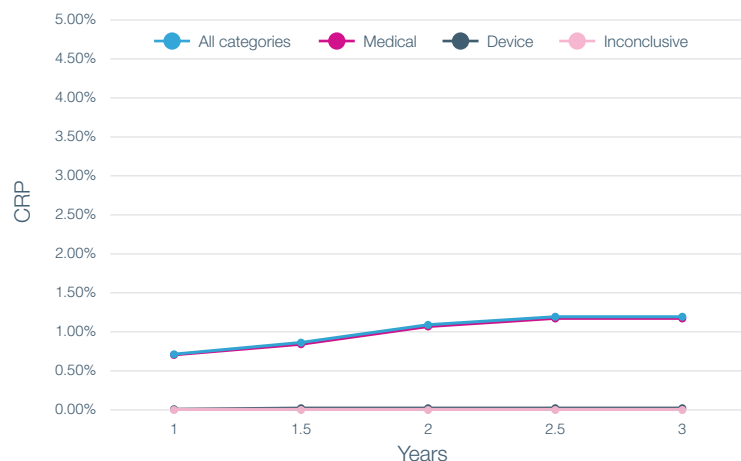


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

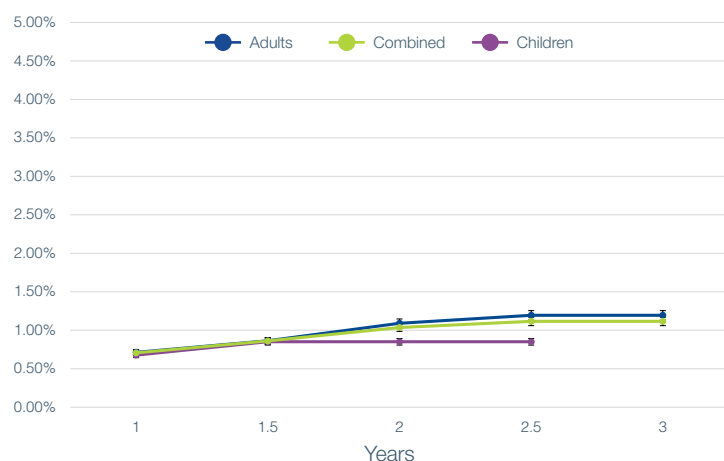

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

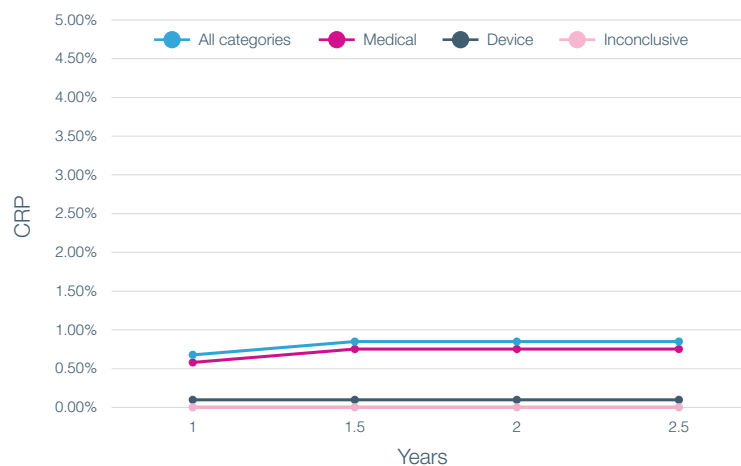

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

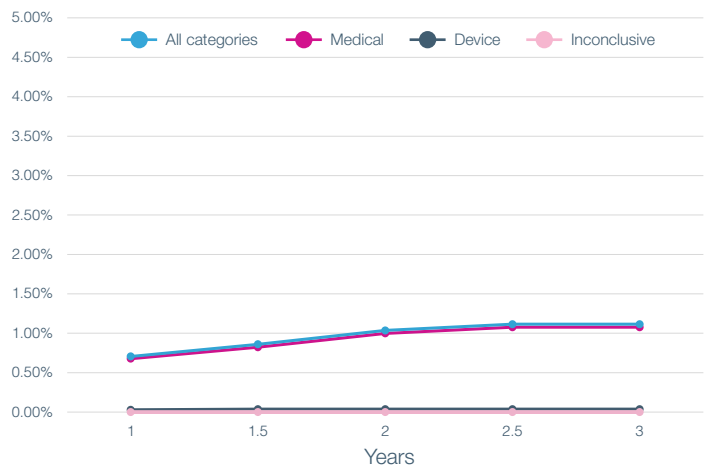

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.68%	0.03%	0.00%	0.71%	0.84%	0.58%
1.5	0.82%	0.04%	0.00%	0.86%	1.01%	0.71%
2	1.00%	0.04%	0.00%	1.04%	1.22%	0.86%
2.5	1.08%	0.04%	0.00%	1.12%	1.32%	0.91%
3	1.08%	0.04%	0.00%	1.12%	1.32%	0.91%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES ULTRA V2

Featuring the proven performance platform as the HiRes 90K™ Advantage, the HiRes Ultra (V2) offers a robust, thin, and discreet mechanical design that is suitable for adults and children.




Number of registered HiRes Ultra V2 implants

As of April 3, 2023.
Date of first commercial introduction: 2019.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	2365	3734	6099 ^b
ANSI/AAMI CI86	2701 ^c	3398	6099

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

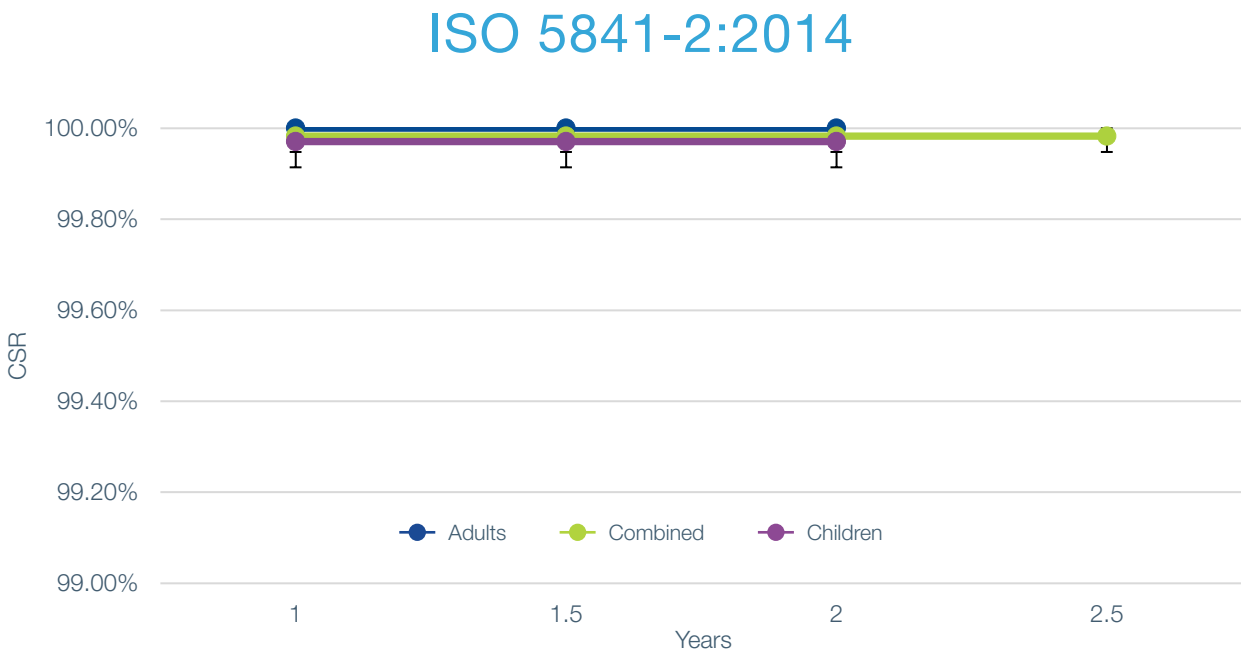


CUMULATIVE SURVIVAL RATE				
Years in use	1	1.5	2	2.5
ADULTS	100.00%	100.00%	100.00%	N/A*
COMBINED	99.98%	99.98%	99.98%	99.98%
CHILDREN	99.97%	99.97%	99.97%	N/A*


*Sample size is not large enough for reporting

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

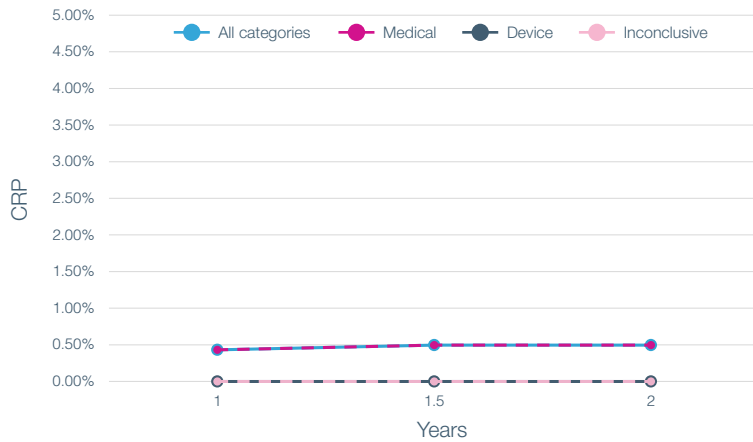


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

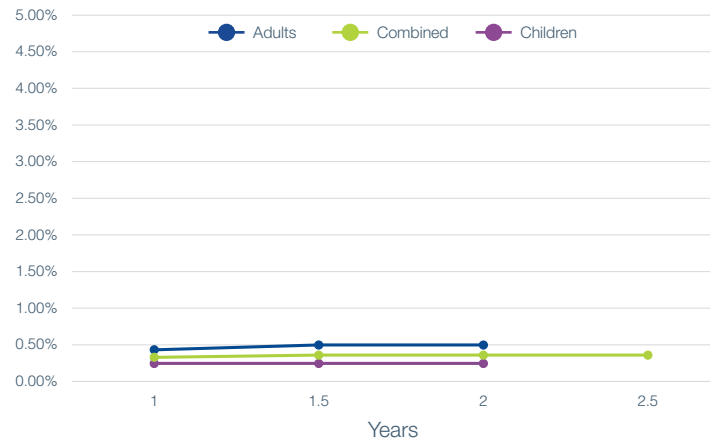

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

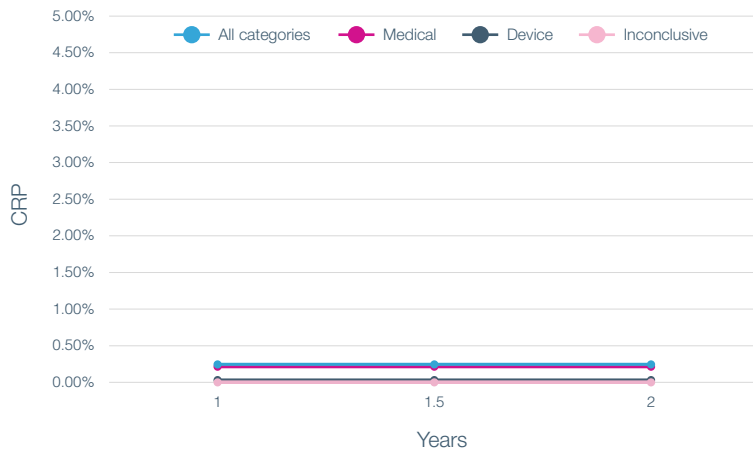

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

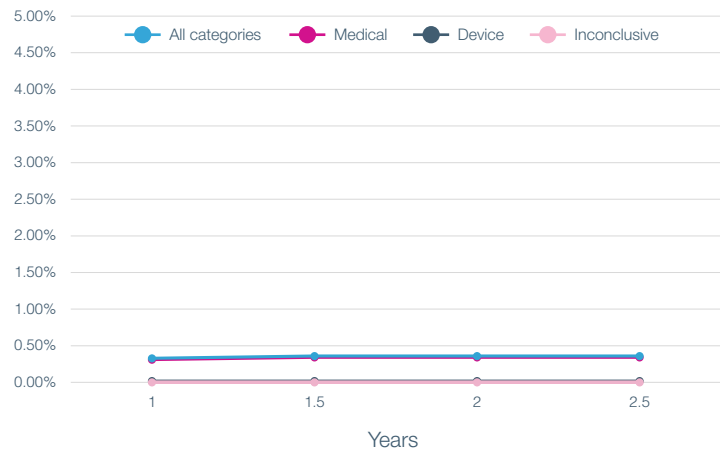

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.31%	0.02%	0.00%	0.33%	0.49%	0.17%
1.5	0.34%	0.02%	0.00%	0.36%	0.53%	0.19%
2	0.34%	0.02%	0.00%	0.36%	0.53%	0.19%
2.5	0.34%	0.02%	0.00%	0.36%	0.53%	0.19%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

PREVIOUS-GENERATION IMPLANT DATA

HIRES ULTRA 3D V1

The HiRes™ Ultra 3D (V1) cochlear implant is an update to the previous HiRes Ultra (V1) device. Advanced Bionics will continue to provide regular reliability updates on the HiRes Ultra platform as new data and information becomes available.

Number of registered HiRes Ultra 3D (V1) implants

As of April 3, 2023.

Last year of distribution: subject to voluntary field action February, 2020.^a


STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	4987	1706	6693 ^b
ANSI/AAMI CI86	5255 ^c	1438	6693

a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.

b. The combined number also includes any registered users for whom we do not have date of birth information.

c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

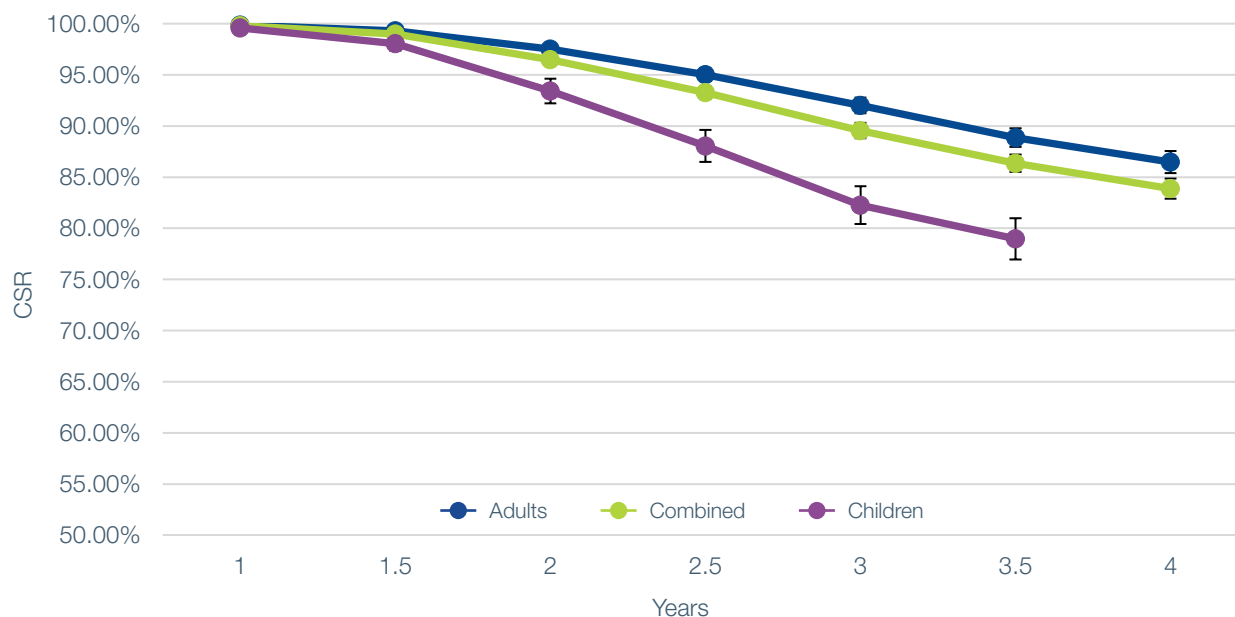


CUMULATIVE SURVIVAL RATE

Years in use	1	1.5	2	2.5	3	3.5	4
ADULTS	99.86%	99.31%	97.53%	95.01%	92.02%	88.86%	86.49%
COMBINED	99.79%	98.99%	96.48%	93.25%	89.55%	86.36%	83.87%
CHILDREN	99.59%	98.04%	93.42%	88.05%	82.26%	78.97%	N/A*


*Sample size is not large enough for reporting

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

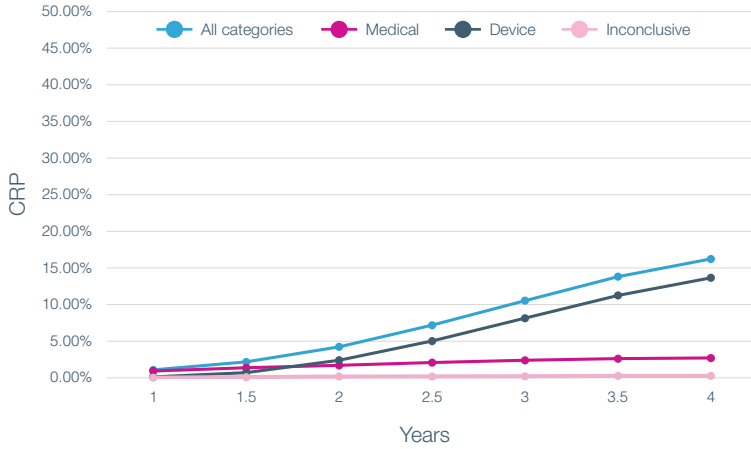


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

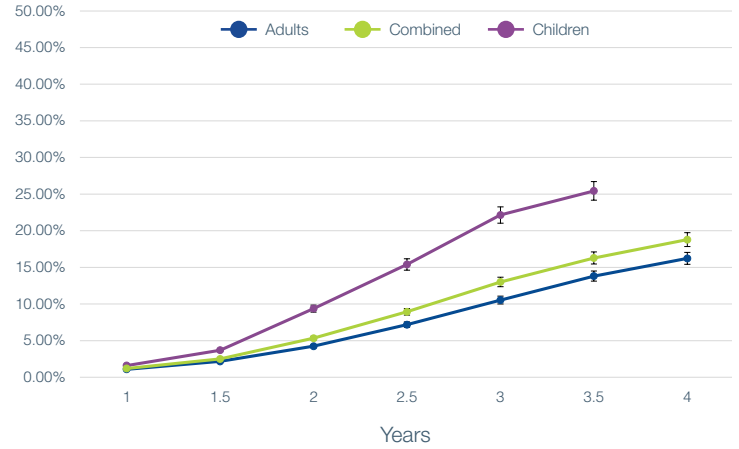

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

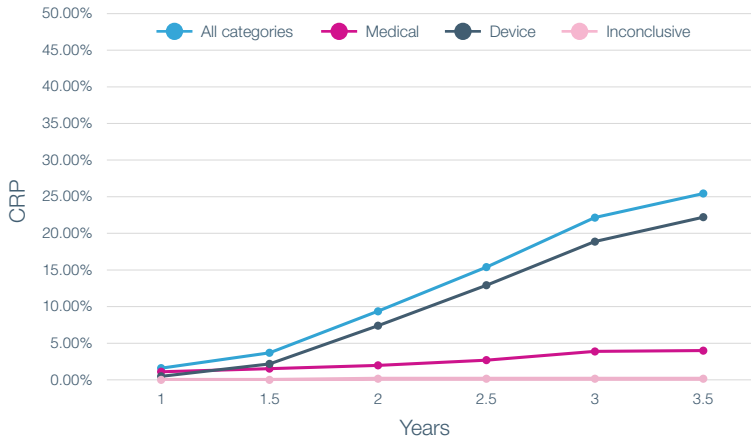

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

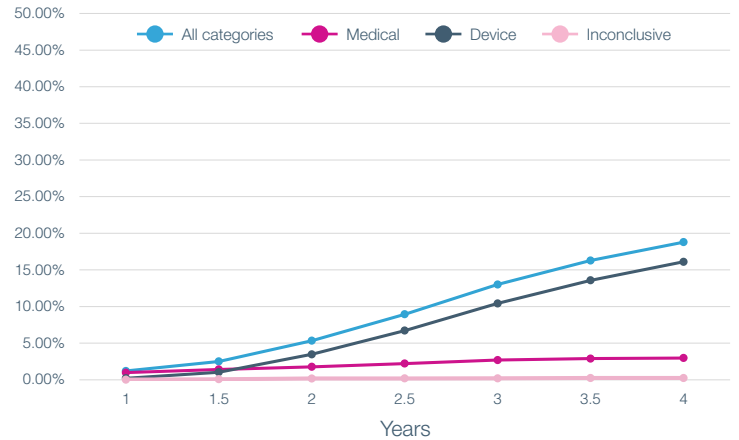

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.97%	0.21%	0.01%	1.20%	1.46%	0.94%
1.5	1.41%	1.03%	0.08%	2.50%	2.87%	2.12%
2	1.76%	3.47%	0.17%	5.34%	5.88%	4.80%
2.5	2.21%	6.71%	0.19%	8.94%	9.62%	8.25%
3	2.69%	10.42%	0.20%	13.01%	13.82%	12.20%
3.5	2.90%	13.58%	0.24%	16.28%	17.19%	15.38%
4	2.97%	16.10%	0.24%	18.79%	19.82%	17.76%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES ULTRA v1

The HiRes™ Ultra (V1) cochlear implant was subject to a Voluntary Field Action initiated by Advanced Bionics in February 2020, and was withdrawn from sale worldwide. This was due to recognition of a common failure mode for a small number of devices, resulting in loss of clinical benefit. Advanced Bionics will continue to provide regular reliability updates on the HiRes Ultra platform as new data and information becomes available.


Number of registered HiRes Ultra (V1) implants

As of April 3, 2023.
Last year of distribution: subject to voluntary field action February, 2020.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	8065	4485	12550 ^b
ANSI/AAMI C186	8624 ^c	3926	12550

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

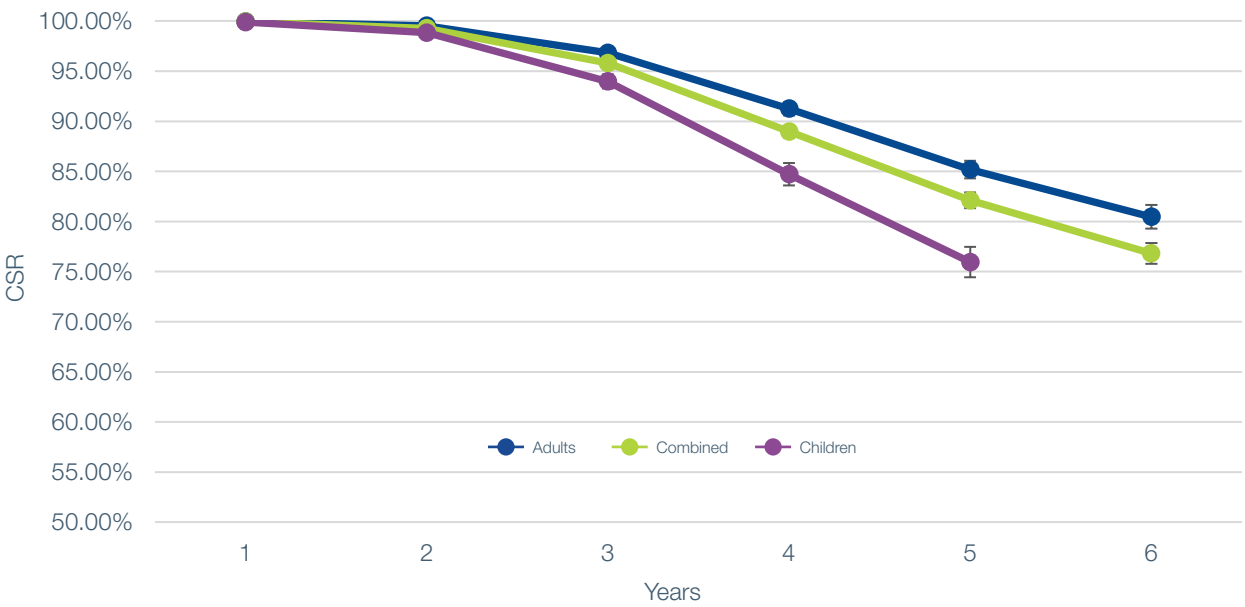


CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6
ADULTS	99.96%	99.52%	96.83%	91.25%	85.19%	80.46%
COMBINED	99.94%	99.27%	95.80%	88.98%	82.11%	76.81%
CHILDREN	99.89%	98.83%	93.97%	84.71%	75.95%	N/A*


*Sample size is not large enough for reporting

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

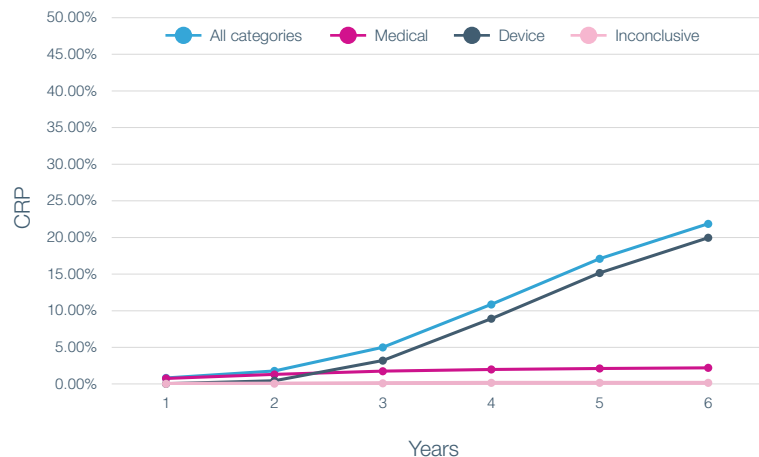


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

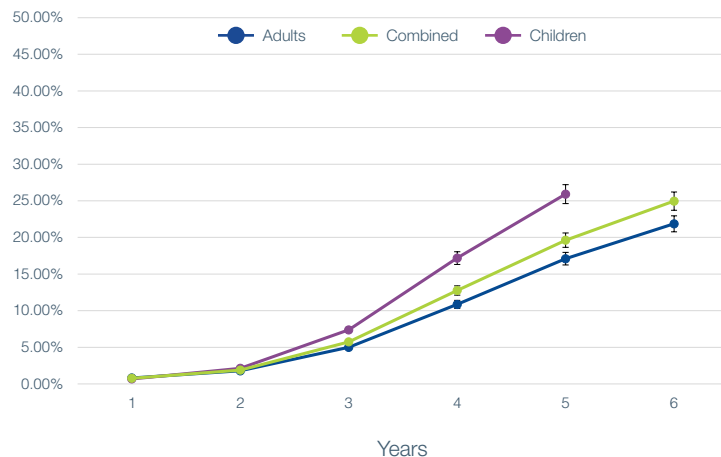

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

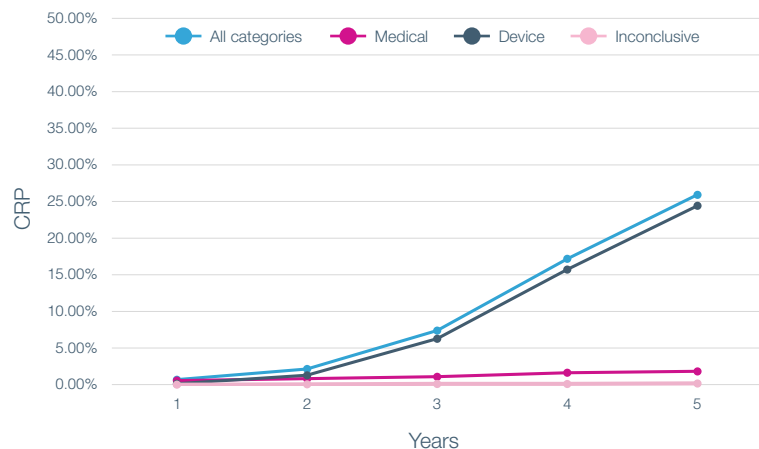

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

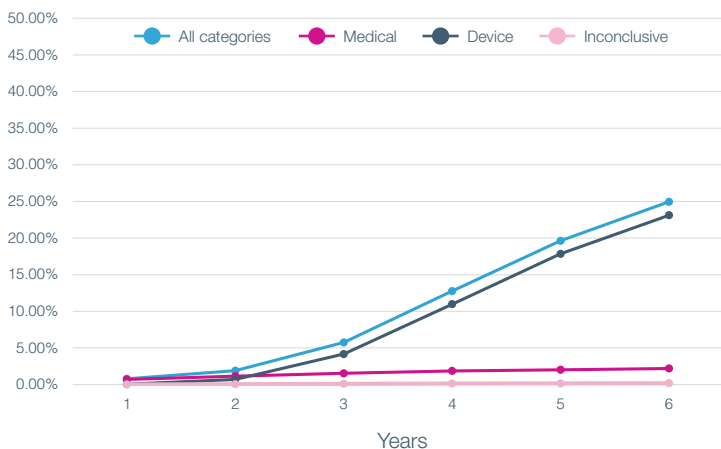

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.70%	0.06%	0.02%	0.78%	0.94%	0.63%
2	1.15%	0.71%	0.05%	1.90%	2.14%	1.66%
3	1.55%	4.17%	0.11%	5.75%	6.16%	5.34%
4	1.87%	10.98%	0.15%	12.77%	13.37%	12.16%
5	2.02%	17.84%	0.16%	19.63%	20.42%	18.84%
6	2.20%	23.12%	0.20%	24.96%	26.00%	23.91%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES 90K ADVANTAGE

The HiRes 90K™ Advantage cochlear implant offers mechanical improvements over its predecessor, the HiRes 90K cochlear implant. It has the capability to offer advanced sound coding strategies, together with the security of a deep bone bed.




Number of registered HiRes 90K Advantage implants

As of April 3, 2023.
Last year of distribution: 2023.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	18225	24409	42634 ^b
ANSI/AAMI C186	20788 ^c	21846	42634

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

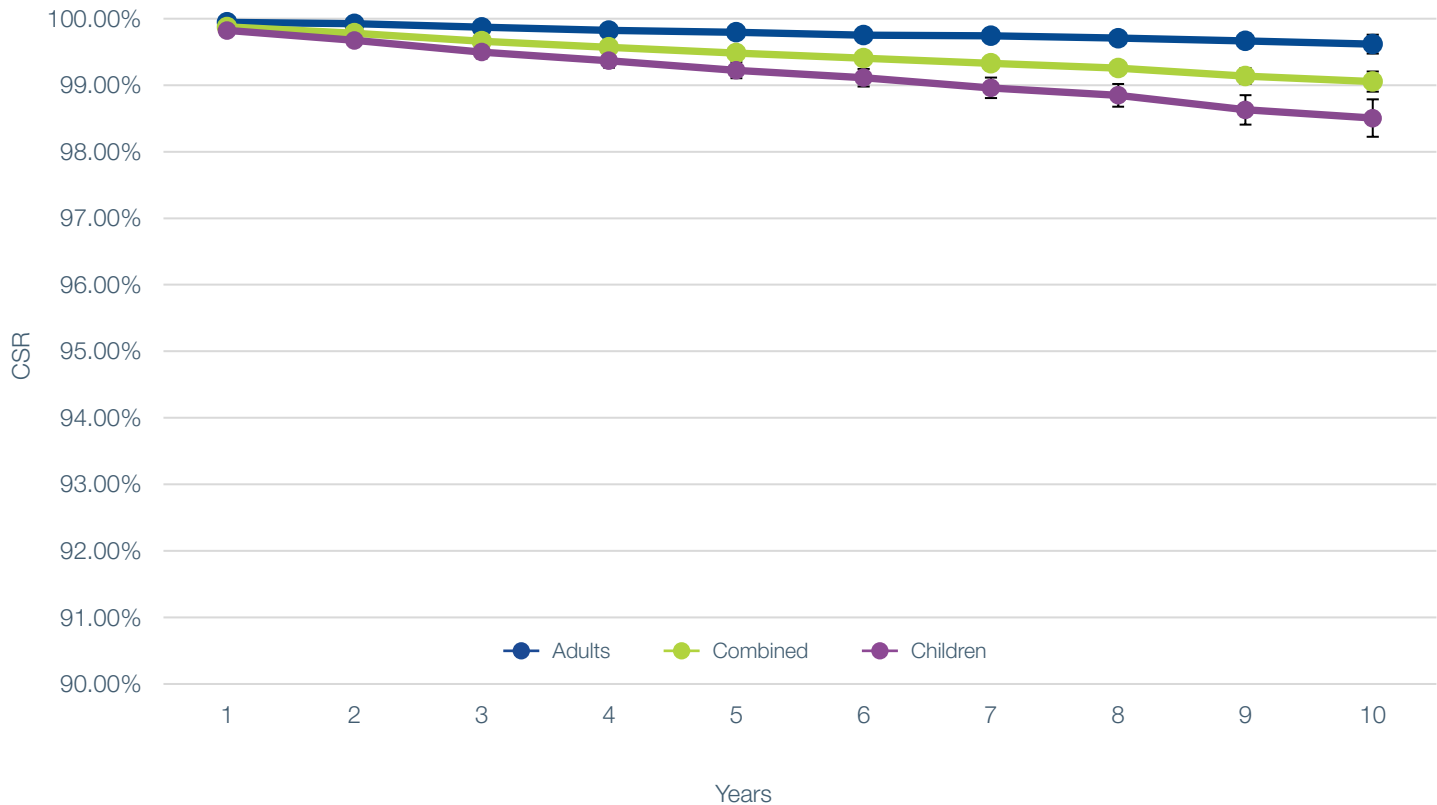


CUMULATIVE SURVIVAL RATE


Years in use	1	2	3	4	5	6	7	8	9	10
ADULTS	99.94%	99.92%	99.87%	99.82%	99.79%	99.75%	99.74%	99.71%	99.67%	99.62%
COMBINED	99.87%	99.78%	99.66%	99.57%	99.48%	99.41%	99.33%	99.26%	99.14%	99.05%
CHILDREN	99.82%	99.67%	99.50%	99.37%	99.22%	99.11%	98.96%	98.85%	98.63%	98.50%

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

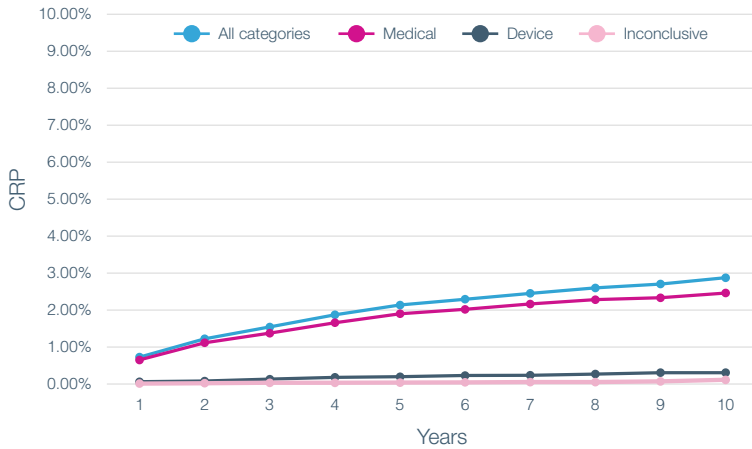


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

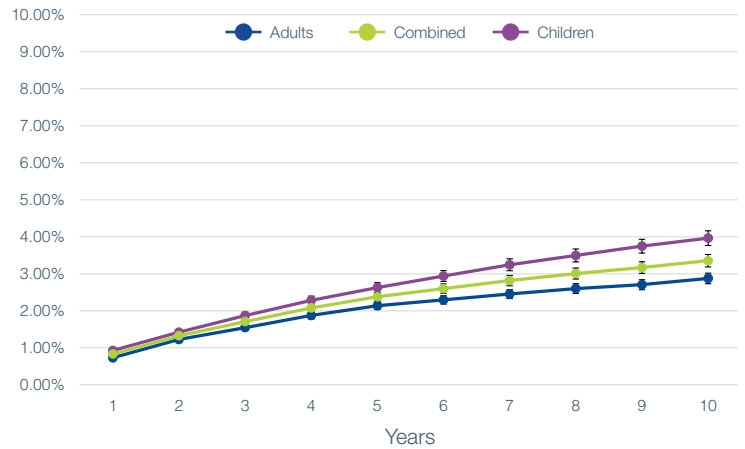

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

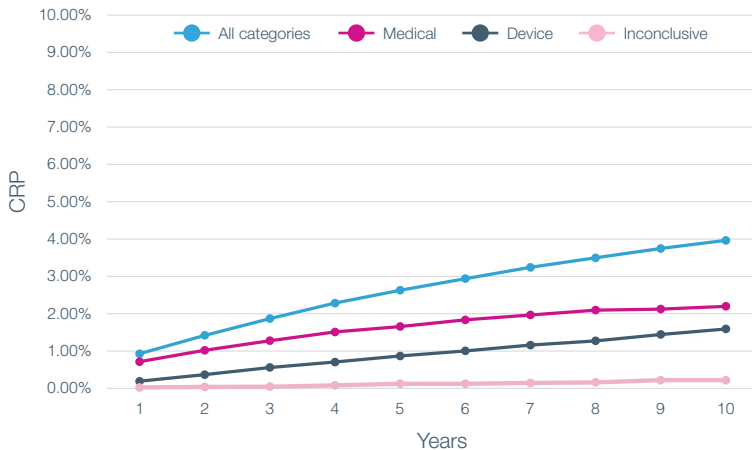

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

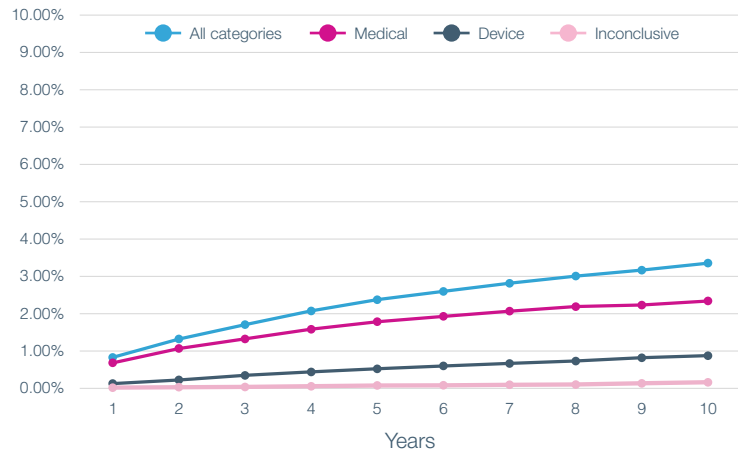

COMBINED ADULT AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.68%	0.13%	0.02%	0.83%	0.92%	0.74%
2	1.07%	0.23%	0.03%	1.32%	1.43%	1.21%
3	1.33%	0.35%	0.04%	1.71%	1.83%	1.58%
4	1.59%	0.44%	0.06%	2.08%	2.22%	1.94%
5	1.79%	0.52%	0.08%	2.38%	2.53%	2.23%
6	1.93%	0.60%	0.08%	2.60%	2.76%	2.44%
7	2.07%	0.67%	0.10%	2.82%	2.99%	2.65%
8	2.19%	0.73%	0.10%	3.01%	3.19%	2.82%
9	2.23%	0.82%	0.14%	3.17%	3.37%	2.97%
10	2.34%	0.88%	0.16%	3.36%	3.60%	3.11%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES 90K vendor A post-mod

The HiRes 90K™ cochlear implant offers access to advanced sound coding technologies. It has undergone manufacturing modifications, with the version currently available being designated as the HiRes 90K (vendor A post-mod) implant.

Number of registered HiRes 90K implants (vendor A post-mod)


As of April 3, 2023.
Last year of distribution: 2018.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	34297	46862	81159 ^b
ANSI/AAMI C186	40202 ^c	40957	81159



- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
- b. The combined number also includes any registered users for whom we do not have date of birth information.
- c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.


ISO 5841-2:2014

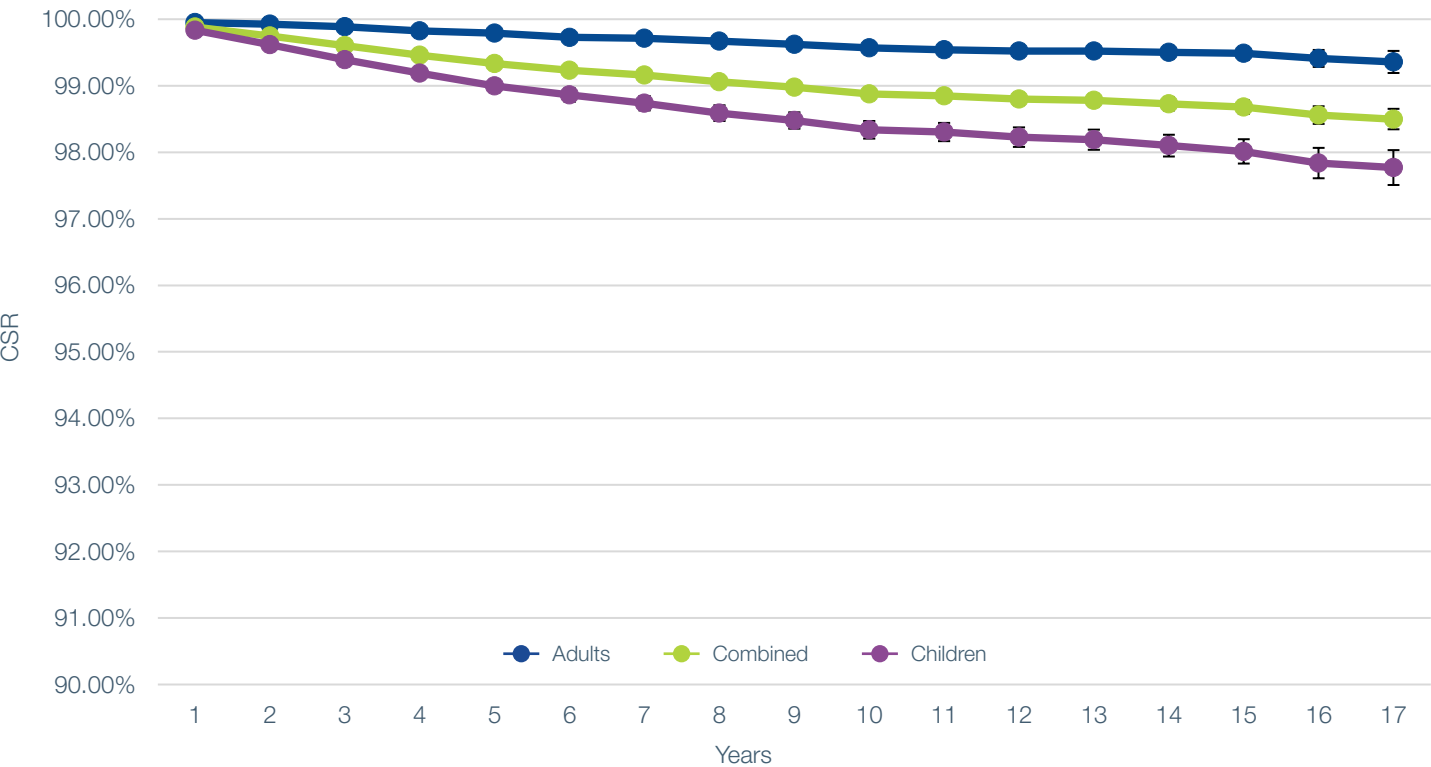


CUMULATIVE SURVIVAL RATE																	
Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17
ADULTS	99.95%	99.93%	99.89%	99.82%	99.79%	99.73%	99.71%	99.67%	99.62%	99.57%	99.54%	99.52%	99.52%	99.50%	99.48%	99.41%	99.36%
COMBINED	99.88%	99.75%	99.60%	99.46%	99.33%	99.23%	99.16%	99.06%	98.98%	98.88%	98.85%	98.80%	98.78%	98.73%	98.68%	98.56%	98.50%
CHILDREN	99.83%	99.62%	99.39%	99.19%	98.99%	98.86%	98.74%	98.59%	98.48%	98.34%	98.30%	98.23%	98.19%	98.10%	98.01%	97.84%	97.77%

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

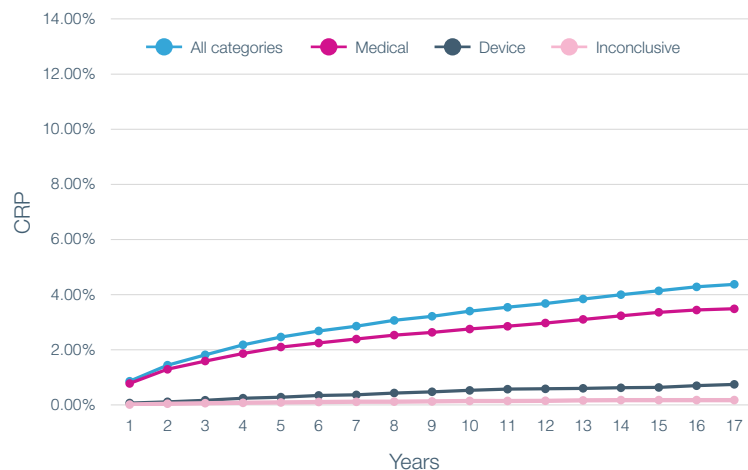


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

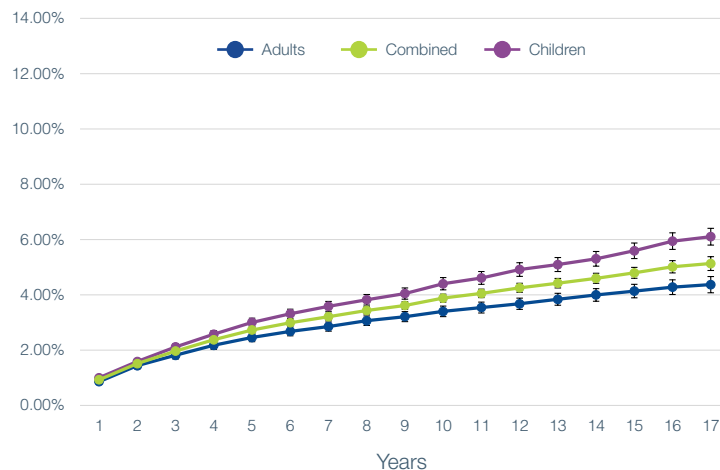

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

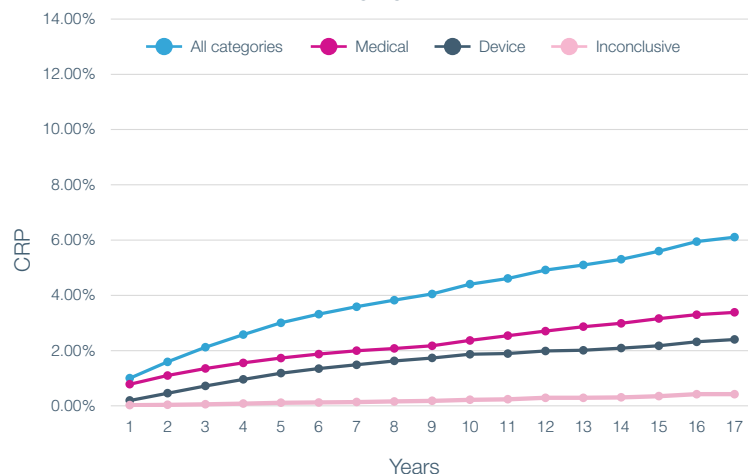

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

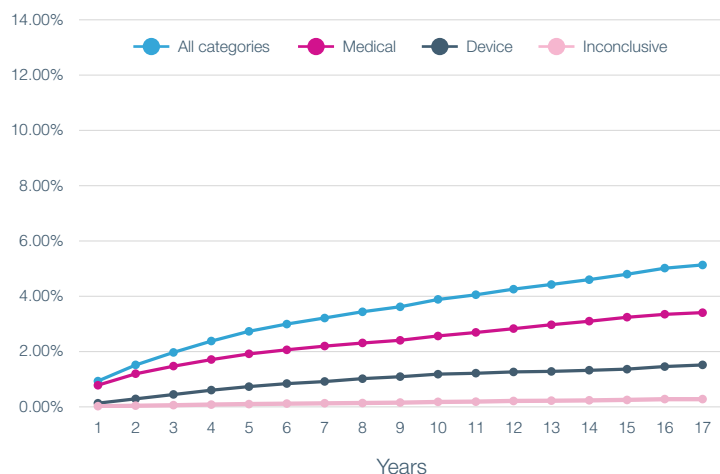

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.78%	0.13%	0.02%	0.93%	1.00%	0.87%
2	1.20%	0.29%	0.04%	1.52%	1.60%	1.43%
3	1.47%	0.45%	0.06%	1.97%	2.06%	1.87%
4	1.71%	0.60%	0.08%	2.38%	2.48%	2.27%
5	1.92%	0.73%	0.10%	2.73%	2.84%	2.62%
6	2.06%	0.84%	0.11%	2.99%	3.11%	2.87%
7	2.19%	0.92%	0.13%	3.21%	3.34%	3.09%
8	2.31%	1.02%	0.14%	3.44%	3.57%	3.31%
9	2.41%	1.09%	0.15%	3.62%	3.76%	3.48%
10	2.56%	1.18%	0.18%	3.88%	4.03%	3.74%
11	2.69%	1.22%	0.19%	4.05%	4.21%	3.90%
12	2.83%	1.26%	0.21%	4.26%	4.42%	4.09%
13	2.97%	1.28%	0.22%	4.42%	4.60%	4.25%
14	3.10%	1.32%	0.23%	4.60%	4.78%	4.42%
15	3.24%	1.36%	0.25%	4.80%	5.00%	4.60%
16	3.35%	1.46%	0.28%	5.02%	5.24%	4.79%
17	3.41%	1.52%	0.28%	5.13%	5.38%	4.88%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES 90K vendor A all


Number of registered HiRes 90K implants (vendor A all)

As of April 3, 2023.
Last year of distribution: 2018.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	35748	47959	83707 ^b
ANSI/AAMI CI86	41863 ^c	41884	83707

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

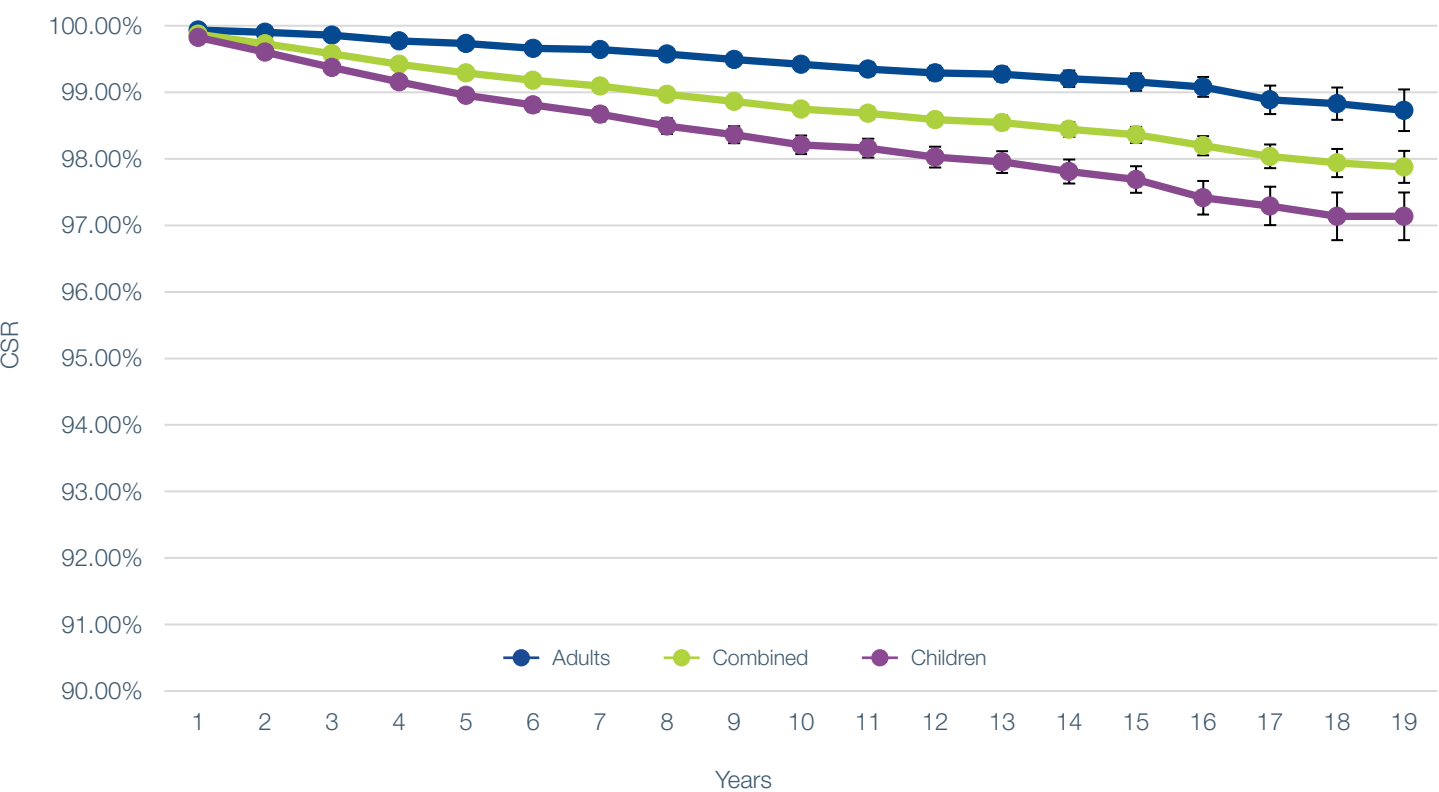


CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10
ADULTS	99.94%	99.90%	99.85%	99.77%	99.73%	99.66%	99.64%	99.57%	99.49%	99.42%
COMBINED	99.87%	99.73%	99.58%	99.42%	99.29%	99.18%	99.09%	98.97%	98.86%	98.75%
CHILDREN	99.83%	99.60%	99.37%	99.16%	98.95%	98.81%	98.67%	98.49%	98.36%	98.21%


Years in use	11	12	13	14	15	16	17	18	19
ADULTS	99.35%	99.29%	99.27%	99.20%	99.15%	99.08%	98.89%	98.83%	98.73%
COMBINED	98.69%	98.59%	98.55%	98.44%	98.36%	98.20%	98.04%	97.94%	97.88%
CHILDREN	98.16%	98.02%	97.95%	97.81%	97.69%	97.41%	97.29%	97.14%	97.14%

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

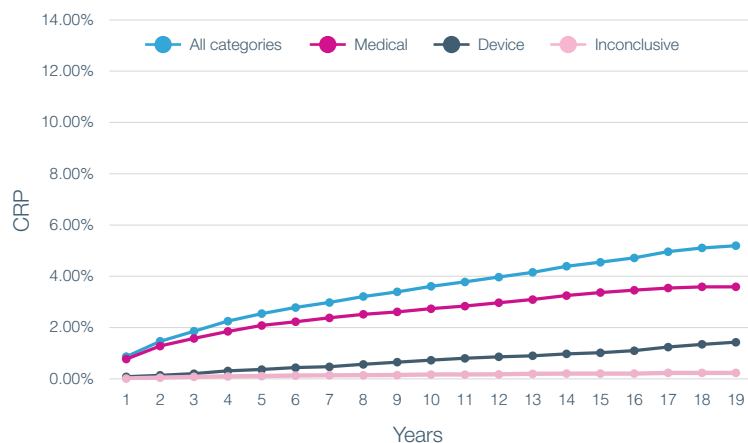


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

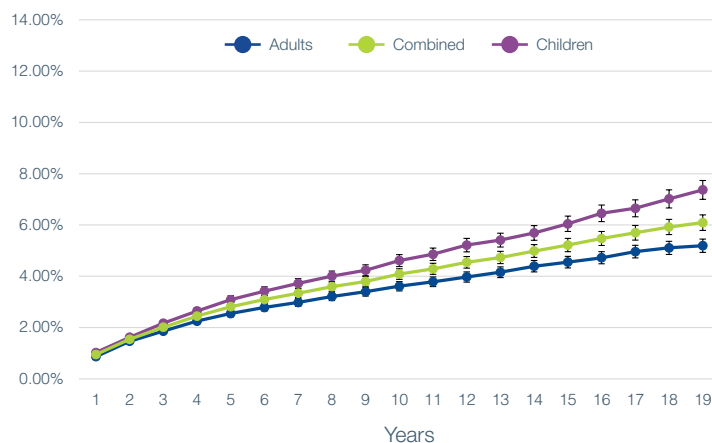

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

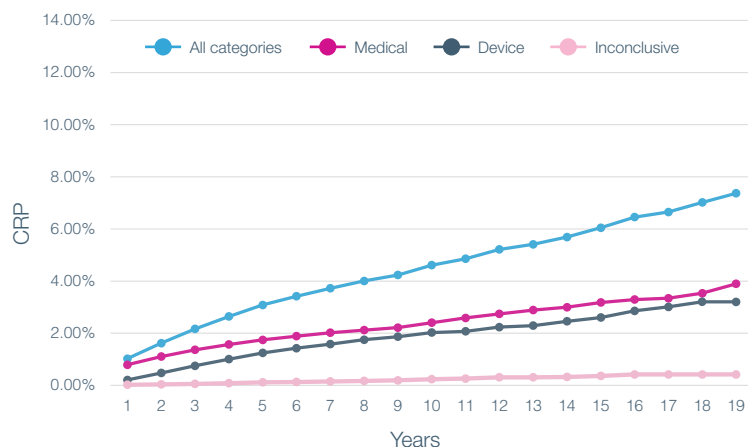

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

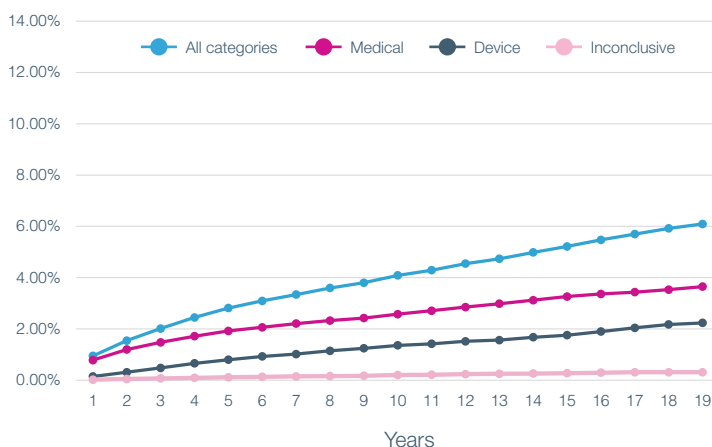

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	Total CI Lower
1	0.78%	0.14%	0.02%	0.95%	1.01%	0.88%
2	1.19%	0.31%	0.04%	1.54%	1.63%	1.46%
3	1.47%	0.48%	0.07%	2.01%	2.11%	1.92%
4	1.71%	0.66%	0.09%	2.45%	2.55%	2.34%
5	1.92%	0.80%	0.11%	2.81%	2.93%	2.70%
6	2.06%	0.92%	0.13%	3.09%	3.21%	2.97%
7	2.21%	1.02%	0.15%	3.34%	3.47%	3.21%
8	2.33%	1.14%	0.16%	3.59%	3.73%	3.46%
9	2.42%	1.24%	0.17%	3.80%	3.94%	3.66%
10	2.57%	1.36%	0.20%	4.09%	4.23%	3.94%
11	2.71%	1.42%	0.21%	4.29%	4.44%	4.13%
12	2.85%	1.52%	0.23%	4.54%	4.71%	4.38%
13	2.98%	1.56%	0.25%	4.73%	4.91%	4.56%
14	3.12%	1.67%	0.26%	4.98%	5.17%	4.80%
15	3.26%	1.75%	0.27%	5.22%	5.42%	5.01%
16	3.36%	1.90%	0.29%	5.47%	5.70%	5.25%
17	3.43%	2.04%	0.31%	5.70%	5.95%	5.44%
18	3.53%	2.17%	0.31%	5.92%	6.22%	5.62%
19	3.65%	2.23%	0.31%	6.09%	6.45%	5.73%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.


HIRES 90K vendor A pre-mod

Number of registered HiRes 90K implants (vendor A pre-mod)

As of April 3, 2023.
Last year of distribution: 2005.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	1451	1097	2548 ^b
ANSI/AAMI CI86	1661 ^c	887	2548


- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

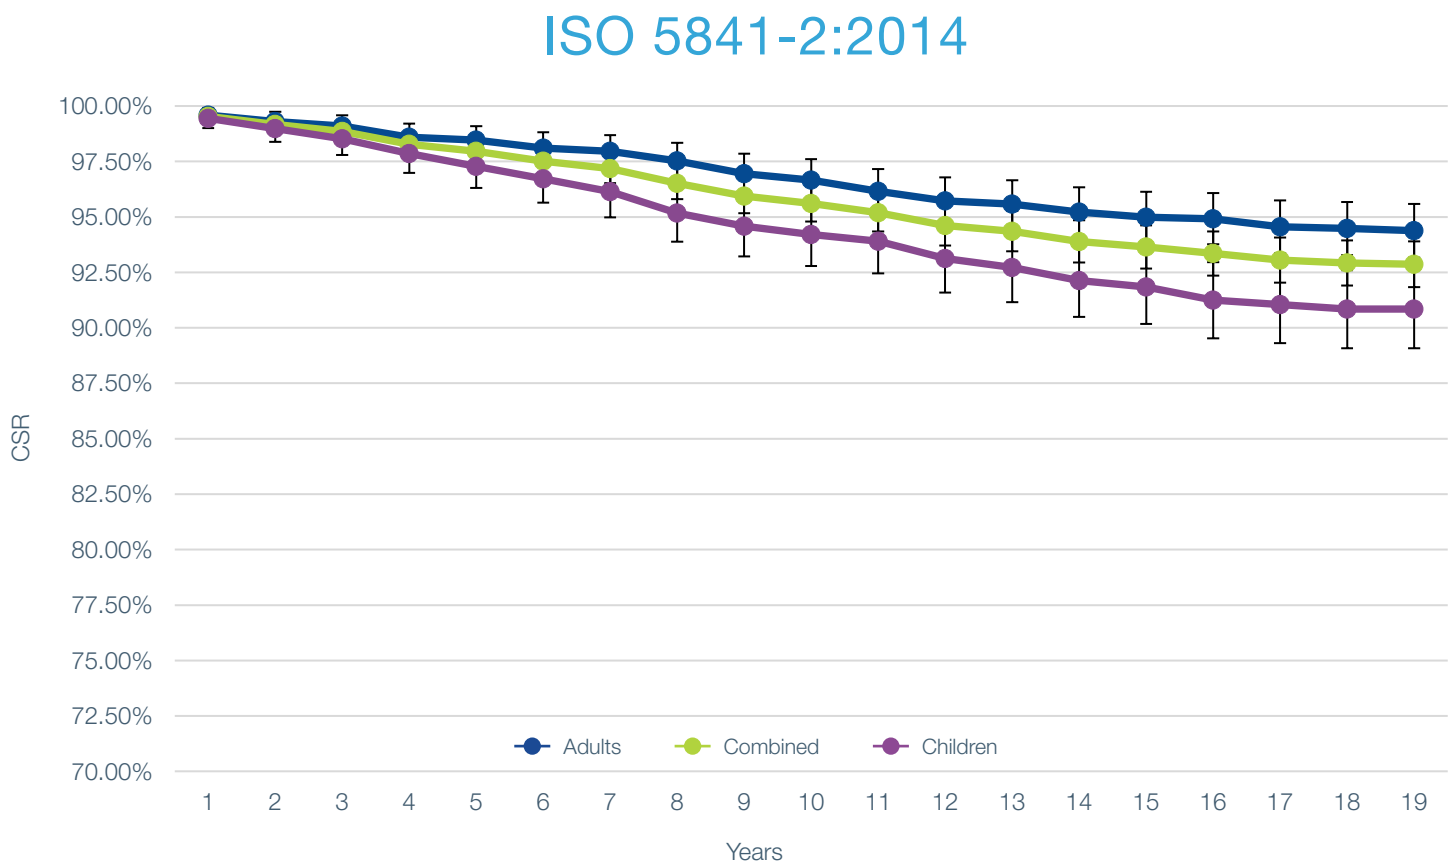


CUMULATIVE SURVIVAL RATE										
Years in use	1	2	3	4	5	6	7	8	9	10
ADULTS	99.59%	99.31%	99.10%	98.60%	98.46%	98.10%	97.96%	97.53%	96.95%	96.66%
COMBINED	99.53%	99.17%	98.85%	98.28%	97.96%	97.51%	97.18%	96.52%	95.94%	95.61%
CHILDREN	99.45%	98.98%	98.52%	97.86%	97.29%	96.71%	96.14%	95.17%	94.59%	94.20%
Years in use	11	12	13	14	15	16	17	18	19	
ADULTS	96.16%	95.72%	95.58%	95.21%	94.99%	94.92%	94.55%	94.48%	94.37%	
COMBINED	95.19%	94.61%	94.36%	93.90%	93.64%	93.35%	93.05%	92.92%	92.86%	
CHILDREN	93.91%	93.12%	92.73%	92.13%	91.84%	91.24%	91.04%	90.84%	90.84%	

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

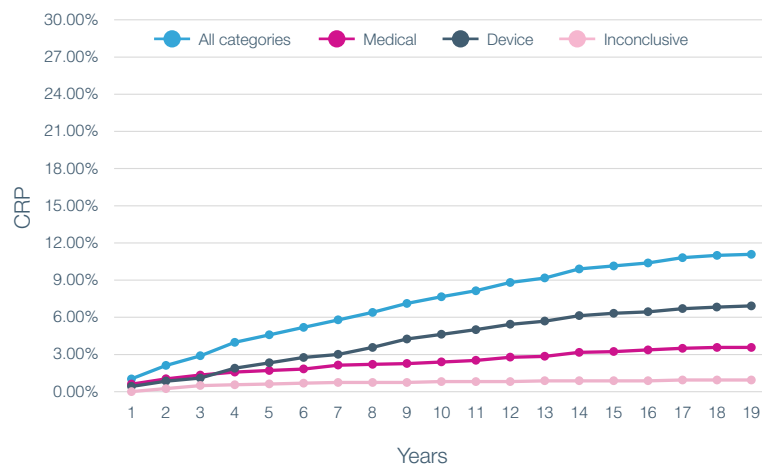


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

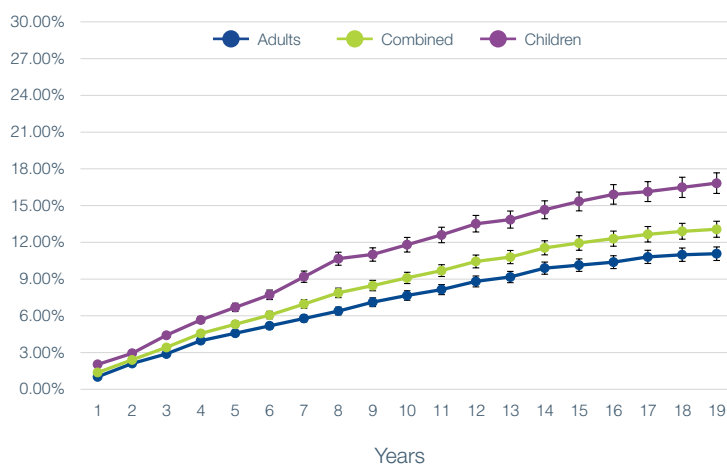

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

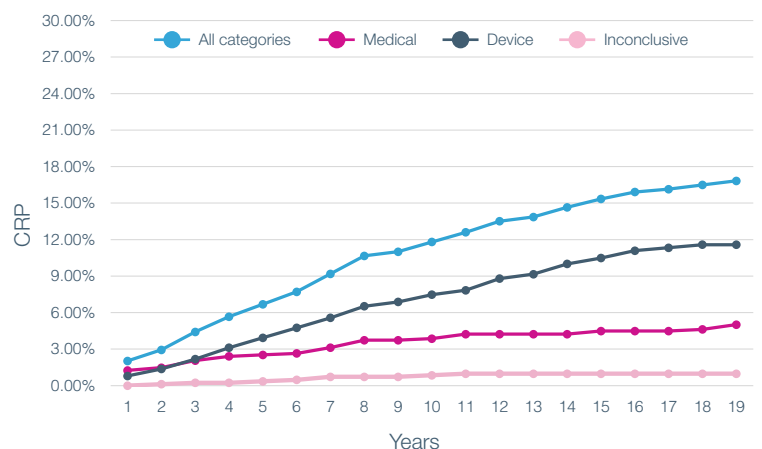

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

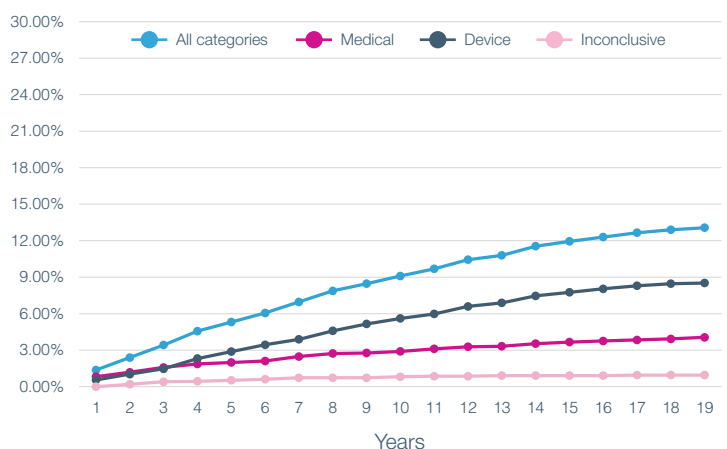

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.83%	0.55%	0.00%	1.37%	1.83%	0.92%
2	1.18%	1.03%	0.20%	2.40%	2.99%	1.80%
3	1.58%	1.47%	0.40%	3.42%	4.13%	2.71%
4	1.87%	2.31%	0.44%	4.56%	5.37%	3.75%
5	1.99%	2.88%	0.53%	5.31%	6.18%	4.44%
6	2.11%	3.45%	0.61%	6.06%	6.99%	5.13%
7	2.48%	3.89%	0.73%	6.97%	7.96%	5.98%
8	2.73%	4.59%	0.73%	7.87%	8.92%	6.83%
9	2.77%	5.16%	0.73%	8.46%	9.55%	7.38%
10	2.90%	5.61%	0.82%	9.10%	10.21%	7.98%
11	3.11%	5.98%	0.86%	9.69%	10.84%	8.54%
12	3.28%	6.60%	0.86%	10.44%	11.63%	9.25%
13	3.32%	6.88%	0.91%	10.80%	12.00%	9.59%
14	3.54%	7.46%	0.91%	11.55%	12.79%	10.30%
15	3.67%	7.75%	0.91%	11.94%	13.20%	10.68%
16	3.75%	8.04%	0.91%	12.30%	13.58%	11.02%
17	3.84%	8.29%	0.95%	12.66%	13.95%	11.36%
18	3.93%	8.46%	0.95%	12.90%	14.20%	11.59%
19	4.05%	8.52%	0.95%	13.07%	14.38%	11.75%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

HIRES 90K vendor B


Number of registered HiRes 90K implants (vendor B)

As of April 3, 2023.
Last year of distribution: subject to voluntary recall in 2006.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	2214	1847	4061 ^b
ANSI/AAMI CI86	2559 ^c	1502	4061

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

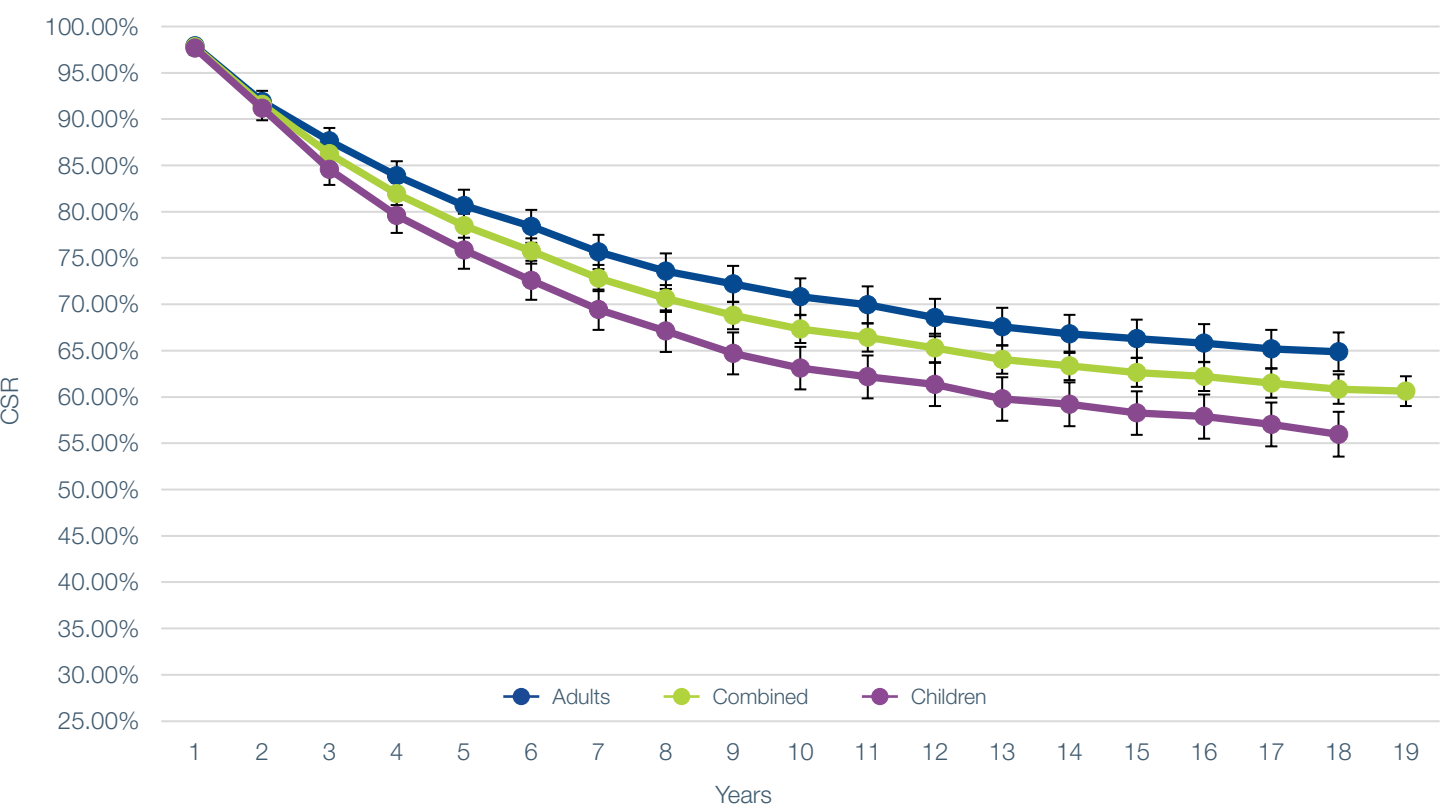


CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10
ADULTS	97.90%	91.91%	87.65%	83.89%	80.67%	78.42%	75.65%	73.58%	72.20%	70.82%
COMBINED	97.79%	91.57%	86.25%	81.94%	78.48%	75.77%	72.82%	70.64%	68.80%	67.32%
CHILDREN	97.65%	91.17%	84.58%	79.61%	75.86%	72.59%	69.43%	67.10%	64.70%	63.10%
Years in use	11	12	13	14	15	16	17	18	19	
ADULTS	69.95%	68.56%	67.58%	66.80%	66.28%	65.81%	65.17%	64.86%	N/A*	
COMBINED	66.42%	65.29%	64.04%	63.36%	62.64%	62.21%	61.48%	60.84%	60.63%	
CHILDREN	62.17%	61.35%	59.78%	59.21%	58.26%	57.88%	57.03%	55.97%	N/A*	


*Sample size is not large enough for reporting

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

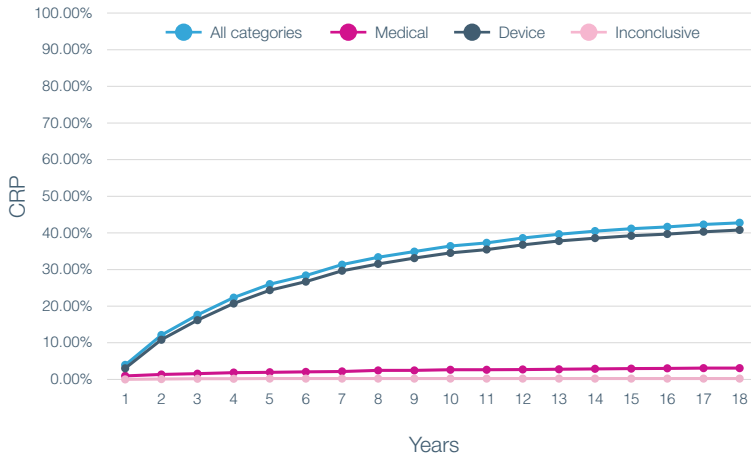


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

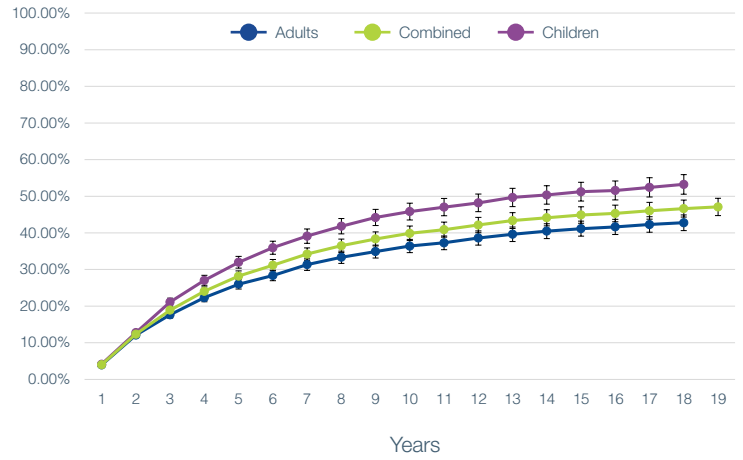

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

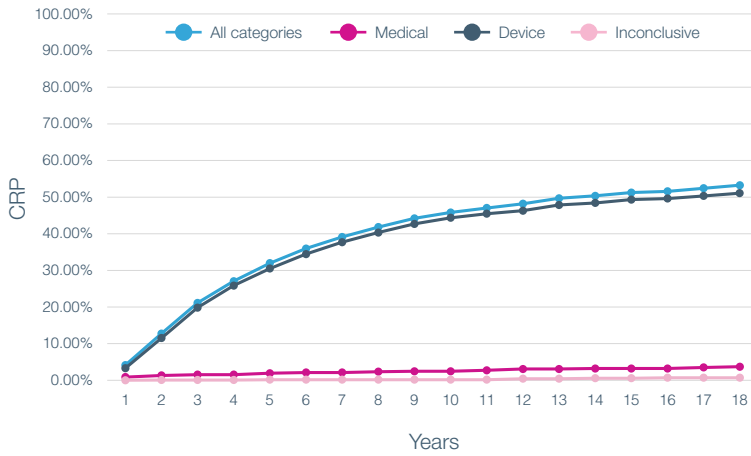

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

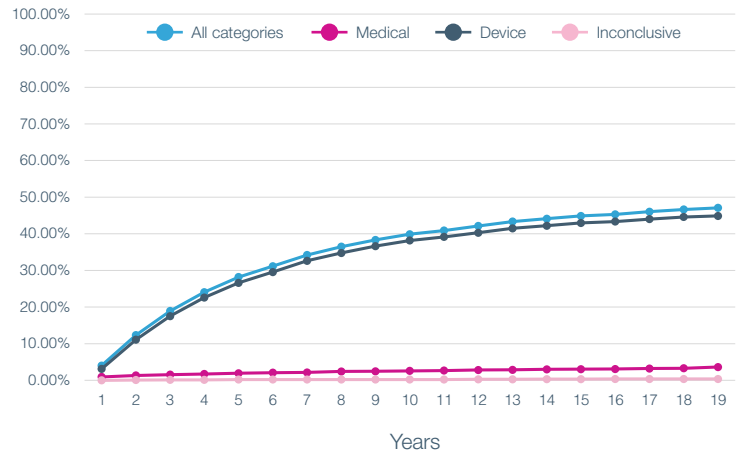

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.93%	3.12%	0.00%	4.02%	4.62%	3.41%
2	1.33%	11.09%	0.08%	12.34%	13.36%	11.33%
3	1.56%	17.53%	0.14%	18.93%	20.13%	17.72%
4	1.74%	22.61%	0.14%	24.07%	25.39%	22.75%
5	1.94%	26.63%	0.21%	28.20%	29.59%	26.81%
6	2.08%	29.56%	0.21%	31.17%	32.60%	29.74%
7	2.15%	32.62%	0.21%	34.21%	35.68%	32.75%
8	2.42%	34.77%	0.21%	36.48%	37.97%	35.00%
9	2.46%	36.65%	0.21%	38.33%	39.84%	36.83%
10	2.58%	38.17%	0.21%	39.89%	41.40%	38.37%
11	2.66%	39.15%	0.21%	40.89%	42.41%	39.37%
12	2.83%	40.28%	0.29%	42.14%	43.67%	40.62%
13	2.87%	41.50%	0.29%	43.35%	44.88%	41.82%
14	3.00%	42.20%	0.34%	44.13%	45.66%	42.59%
15	3.04%	42.96%	0.34%	44.88%	46.42%	43.34%
16	3.09%	43.35%	0.38%	45.31%	46.85%	43.77%
17	3.22%	44.02%	0.38%	46.03%	47.57%	44.49%
18	3.29%	44.60%	0.38%	46.63%	48.19%	45.08%
19	3.63%	44.89%	0.38%	47.09%	48.68%	45.50%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

CII BIONIC EAR

The CII Bionic Ear cochlear implant is the base for the advanced technology found in Advanced Bionics implants today. The platform can still take advantage of the latest innovations today. It benefited from the mechanical improvement made to the earlier C1.2 implants.




Number of registered CII implants

As of April 3, 2023.
Last year of distribution: 2004.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	3017	2094	5111 ^b
ANSI/AAMI CI86	3394 ^c	1717	5111

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.
c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

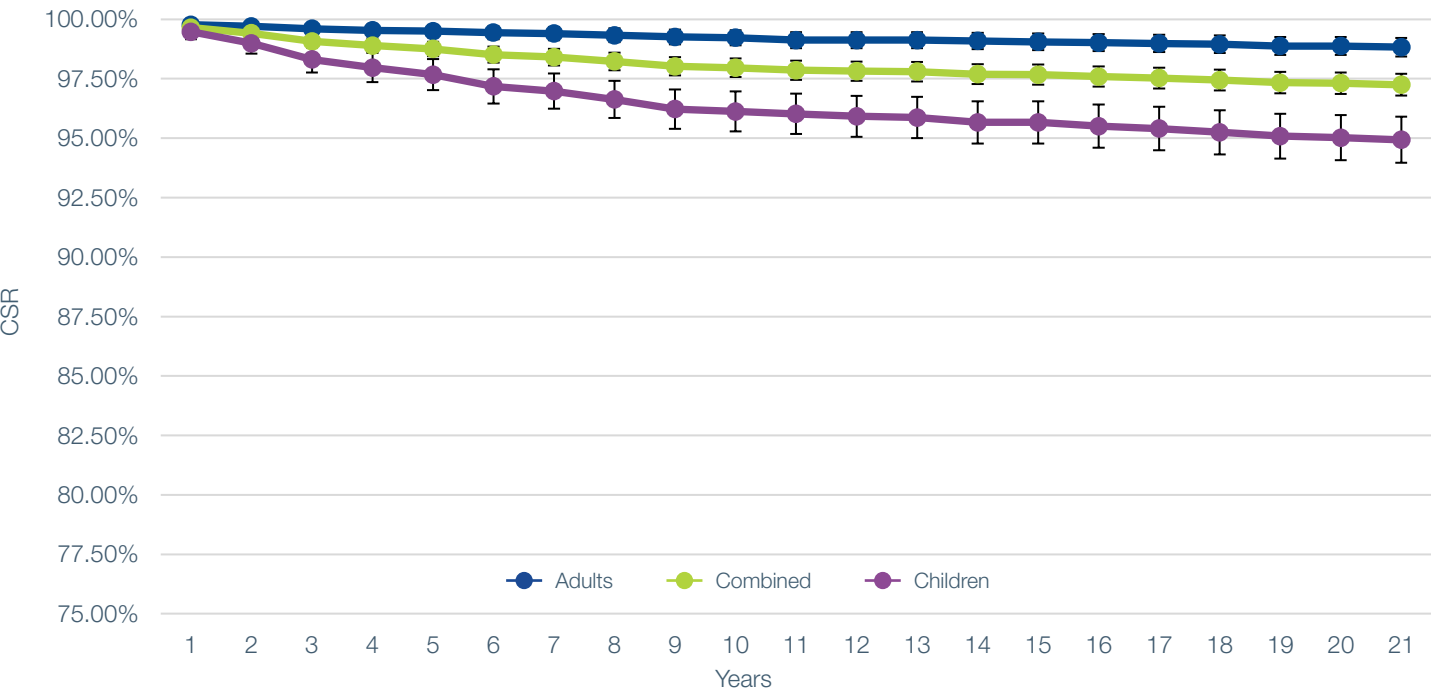


CUMULATIVE SURVIVAL RATE


Years in use	1	2	3	4	5	6	7	8	9	10	11
ADULTS	99.77%	99.70%	99.60%	99.53%	99.50%	99.43%	99.40%	99.33%	99.26%	99.22%	99.12%
COMBINED	99.65%	99.41%	99.07%	98.89%	98.75%	98.51%	98.41%	98.23%	98.02%	97.96%	97.86%
CHILDREN	99.47%	98.99%	98.31%	97.97%	97.67%	97.18%	96.98%	96.63%	96.22%	96.12%	96.02%
Years in use	12	13	14	15	16	17	18	19	20	21	
ADULTS	99.12%	99.12%	99.09%	99.05%	99.02%	98.98%	98.95%	98.88%	98.88%	98.83%	
COMBINED	97.82%	97.80%	97.69%	97.67%	97.59%	97.53%	97.44%	97.34%	97.31%	97.25%	
CHILDREN	95.92%	95.87%	95.66%	95.66%	95.51%	95.40%	95.25%	95.09%	95.02%	94.93%	

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

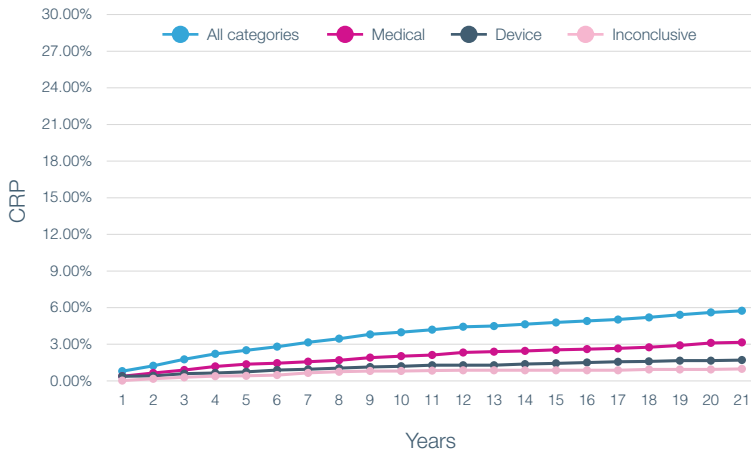


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

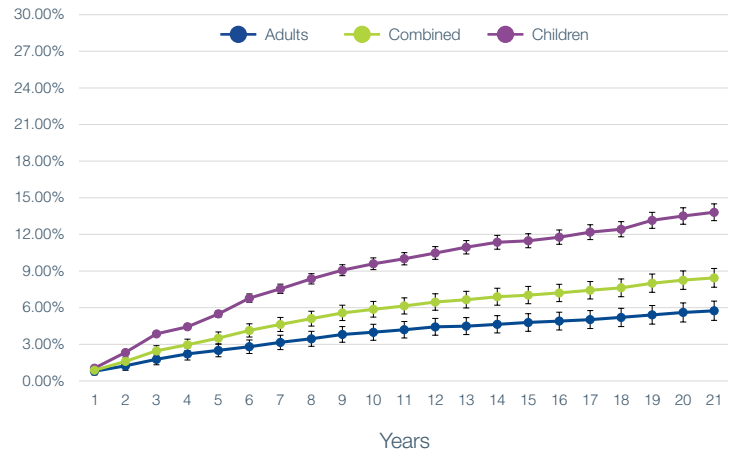

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

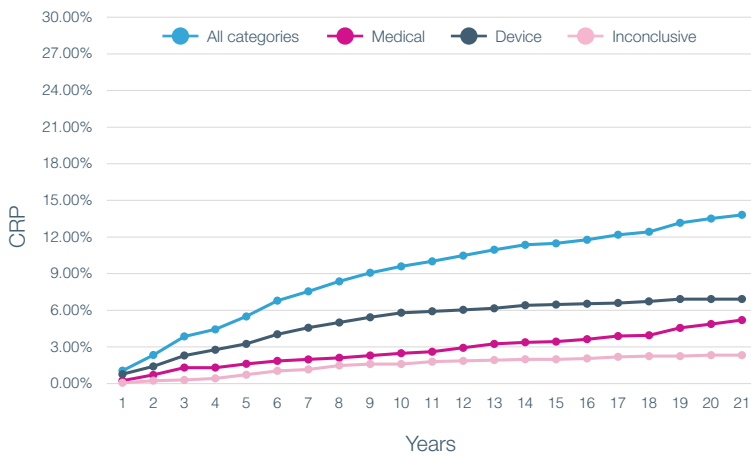

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

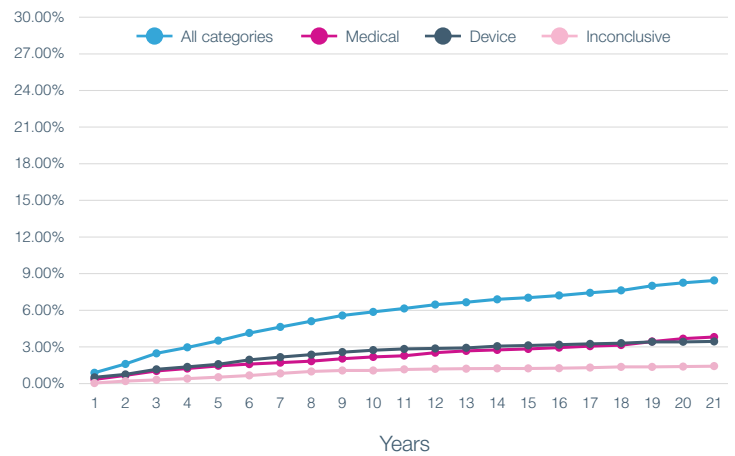

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.33%	0.51%	0.04%	0.88%	1.14%	0.62%
2	0.67%	0.75%	0.20%	1.61%	1.95%	1.26%
3	1.03%	1.16%	0.30%	2.47%	2.89%	2.04%
4	1.23%	1.36%	0.40%	2.96%	3.42%	2.49%
5	1.45%	1.58%	0.52%	3.51%	4.01%	3.00%
6	1.59%	1.94%	0.66%	4.14%	4.68%	3.59%
7	1.71%	2.16%	0.82%	4.63%	5.21%	4.05%
8	1.83%	2.37%	0.99%	5.10%	5.71%	4.50%
9	2.03%	2.57%	1.07%	5.57%	6.20%	4.94%
10	2.18%	2.73%	1.07%	5.87%	6.52%	5.22%
11	2.28%	2.83%	1.15%	6.15%	6.81%	5.49%
12	2.53%	2.88%	1.20%	6.46%	7.14%	5.79%
13	2.67%	2.92%	1.22%	6.66%	7.34%	5.97%
14	2.75%	3.06%	1.24%	6.89%	7.59%	6.20%
15	2.83%	3.12%	1.24%	7.03%	7.74%	6.33%
16	2.94%	3.18%	1.26%	7.21%	7.92%	6.50%
17	3.06%	3.25%	1.30%	7.43%	8.15%	6.71%
18	3.14%	3.31%	1.36%	7.63%	8.35%	6.90%
19	3.44%	3.41%	1.36%	8.01%	8.75%	7.26%
20	3.68%	3.41%	1.39%	8.25%	9.01%	7.50%
21	3.81%	3.45%	1.42%	8.44%	9.21%	7.67%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

CLARION 1.2

The Clarion 1.2 (C1.2) implant offers mechanical improvements over its predecessor the C1.0 implant, which first introduced independent current-sources, a key technology differentiator for Advanced Bionics implants.




Number of registered C1.2 implants

As of April 3, 2023.
Last year of distribution: 2004.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	4237	4157	8484 ^b
ANSI/AAMI C186	4960 ^c	3524	8484

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
- b. The combined number also includes any registered users for whom we do not have date of birth information.
- c. The adult number also includes users whose personal information is not available or may not be obtainable due to certain privacy laws in certain countries.

ISO 5841-2:2014

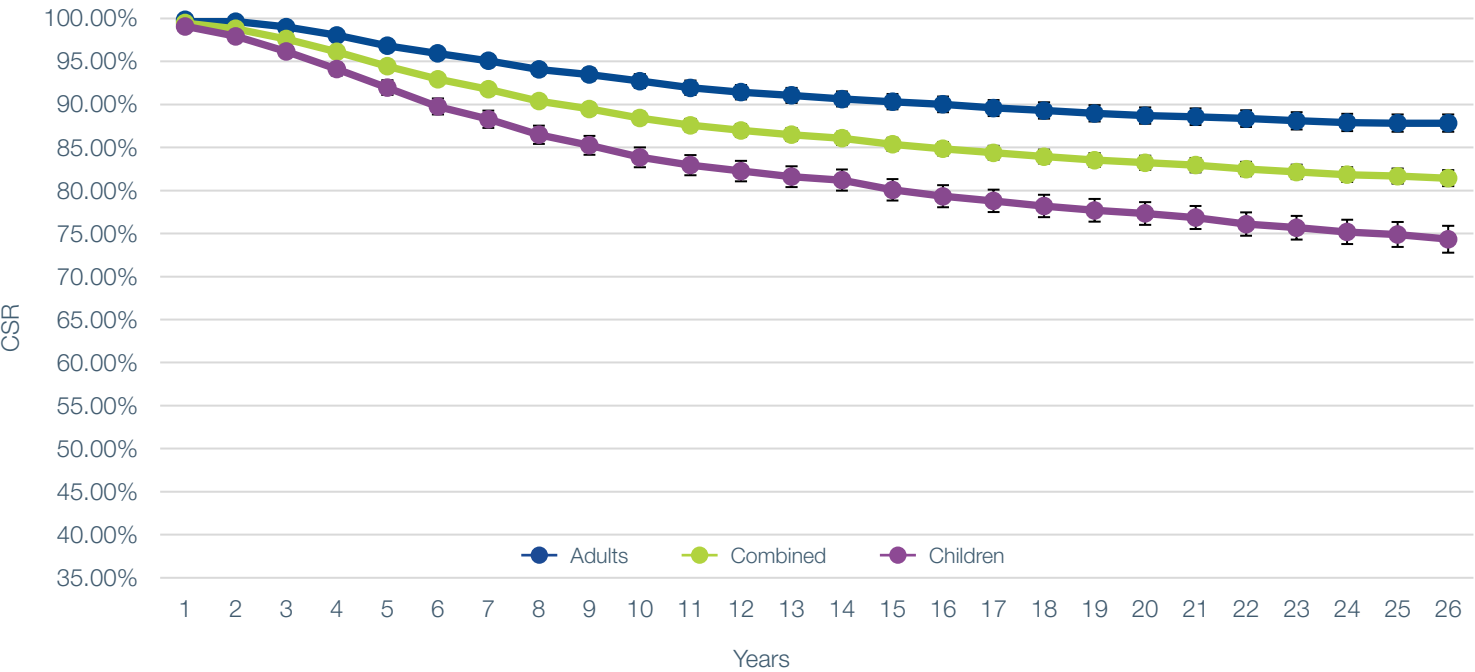


CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13
ADULTS	99.84%	99.63%	98.99%	98.03%	96.82%	95.94%	95.08%	94.07%	93.47%	92.72%	91.94%	91.43%	91.06%
COMBINED	99.47%	98.80%	97.61%	96.12%	94.45%	92.93%	91.77%	90.38%	89.48%	88.42%	87.58%	86.98%	86.48%
CHILDREN	99.08%	97.93%	96.15%	94.11%	91.96%	89.76%	88.28%	86.48%	85.26%	83.86%	82.96%	82.26%	81.61%


Years in use	14	15	16	17	18	19	20	21	22	23	24	25	26
ADULTS	90.64%	90.32%	90.02%	89.60%	89.29%	88.96%	88.71%	88.57%	88.35%	88.09%	87.90%	87.83%	87.83%
COMBINED	86.07%	85.37%	84.86%	84.38%	83.94%	83.54%	83.23%	82.94%	82.49%	82.16%	81.84%	81.67%	81.43%
CHILDREN	81.20%	80.08%	79.33%	78.79%	78.19%	77.70%	77.34%	76.86%	76.10%	75.68%	75.19%	74.89%	74.35%

ANSI/AAMI CI86


REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS

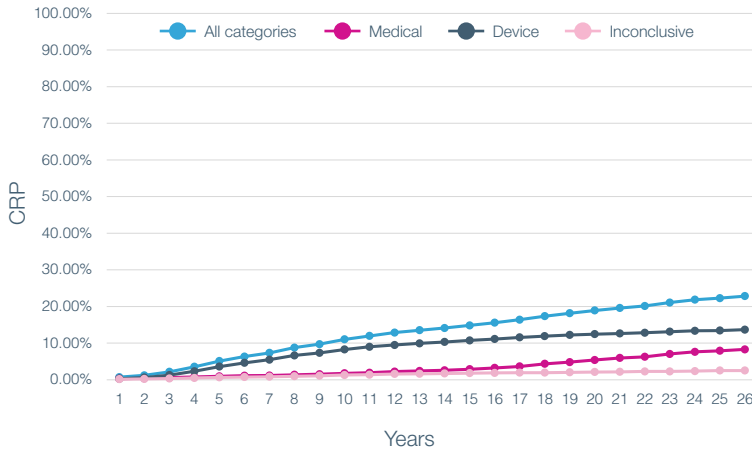


REMOVAL RATES ANALYSIS FOR ALL ANALYSIS CATEGORIES AND DIFFERENT PATIENTS POPULATION

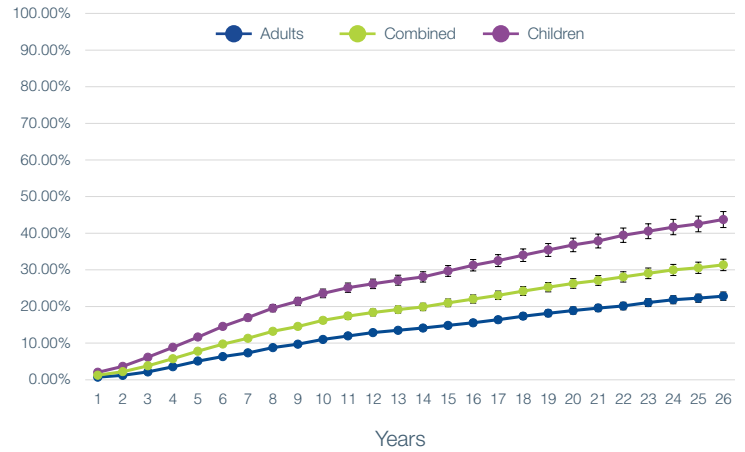

REMOVAL RATES ANALYSIS CATEGORIES FOR CHILDREN

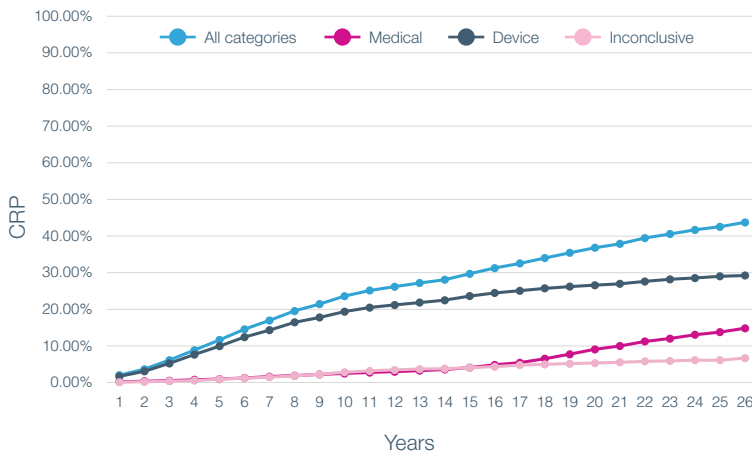

REMOVAL RATES ANALYSIS CATEGORIES FOR ADULTS AND CHILDREN

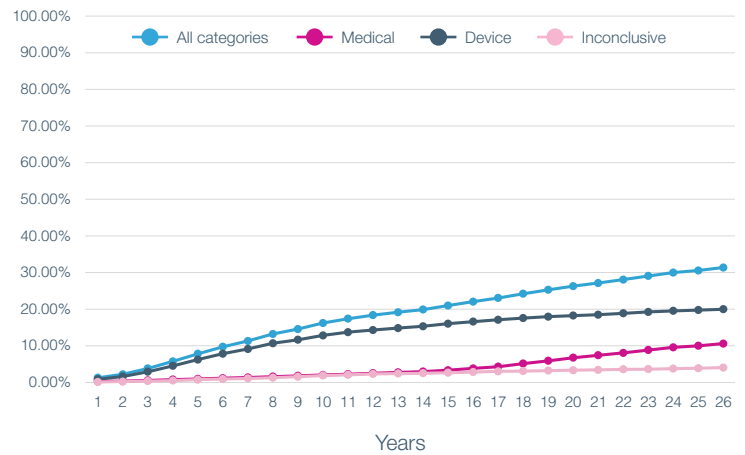

COMBINED ADULTS AND CHILDREN

Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
					CI Higher	CI Lower
1	0.26%	0.86%	0.13%	1.25%	1.49%	1.02%
2	0.38%	1.63%	0.21%	2.21%	2.52%	1.90%
3	0.55%	2.92%	0.36%	3.80%	4.21%	3.39%
4	0.78%	4.52%	0.51%	5.74%	6.24%	5.25%
5	0.94%	6.22%	0.75%	7.80%	8.38%	7.23%
6	1.16%	7.83%	0.92%	9.74%	10.37%	9.10%
7	1.34%	9.12%	1.08%	11.31%	11.99%	10.64%
8	1.57%	10.68%	1.29%	13.23%	13.95%	12.50%
9	1.79%	11.63%	1.54%	14.55%	15.31%	13.80%
10	2.04%	12.83%	1.88%	16.21%	17.00%	15.42%
11	2.24%	13.72%	2.07%	17.40%	18.21%	16.59%
12	2.51%	14.30%	2.30%	18.37%	19.20%	17.54%
13	2.73%	14.83%	2.42%	19.15%	20.00%	18.31%
14	2.96%	15.31%	2.52%	19.89%	20.74%	19.03%
15	3.33%	16.03%	2.65%	20.97%	21.85%	20.10%
16	3.83%	16.58%	2.82%	22.04%	22.92%	21.15%
17	4.30%	17.10%	3.02%	23.05%	23.96%	22.15%
18	5.14%	17.56%	3.09%	24.22%	25.13%	23.30%
19	5.89%	17.96%	3.22%	25.27%	26.21%	24.34%
20	6.74%	18.23%	3.33%	26.28%	27.23%	25.34%
21	7.42%	18.48%	3.43%	27.12%	28.08%	26.16%
22	8.05%	18.86%	3.59%	28.06%	29.03%	27.10%
23	8.84%	19.25%	3.63%	29.06%	30.05%	28.07%
24	9.57%	19.54%	3.76%	29.98%	30.99%	28.96%
25	10.00%	19.75%	3.86%	30.56%	31.60%	29.52%
26	10.60%	19.98%	4.04%	31.36%	32.48%	30.23%

Not all data may be shown alongside the graphs due to space limitations. Please see the **Appendix** at the end of the report for a complete data set.

CLARION 1.0

The Clarion 1.0 (C1.0) implant was Advanced Bionics first device, the start of a technology-forward lineage that continues today. As the number of children implanted with the C1.0 is below the level required for statistical analysis, the data is included in the combined data.




Number of registered C1.0 implants

As of April 3, 2023.
Last year of distribution: 1997.^a

STANDARD	ADULTS	CHILDREN	COMBINED
ISO 5841-2:2014	294	50	344 ^b
ANSI/AAMI C186	–	–	–

- a. Dates provided are those for major markets covered by FDA and TUV regulation. Some implants may be pending approval in a subset of additional regions.
b. The combined number also includes any registered users for whom we do not have date of birth information.

ISO 5841-2:2014

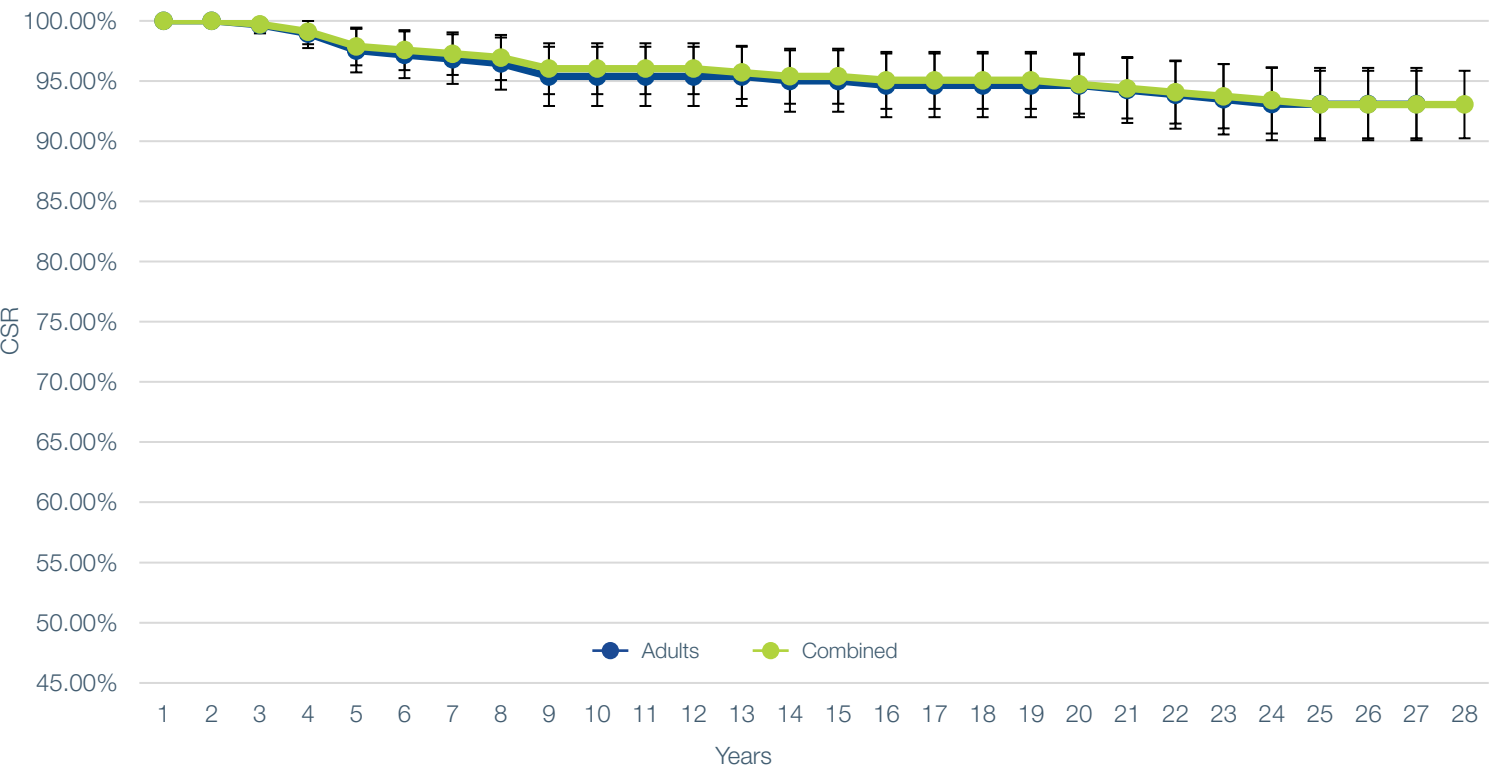

CUMULATIVE SURVIVAL RATE

Years in use	1	2	3	4	5	6	7	8	9	10	11	12	13	14
ADULTS	100.00%	100.00%	99.65%	98.94%	97.52%	97.16%	96.81%	96.45%	95.37%	95.37%	95.37%	95.37%	95.37%	95.00%
COMBINED	100.00%	100.00%	99.70%	99.09%	97.87%	97.56%	97.25%	96.94%	96.02%	96.02%	96.02%	96.02%	95.70%	95.38%

Years in use	15	16	17	18	19	20	21	22	23	24	25	26	27	28
ADULTS	95.00%	94.63%	94.63%	94.63%	94.63%	94.63%	94.24%	93.86%	93.47%	93.08%	93.08%	93.08%	93.08%	N/A
COMBINED	95.38%	95.05%	95.05%	95.05%	95.05%	94.72%	94.39%	94.06%	93.72%	93.38%	93.04%	93.04%	93.04%	93.04%

^aSample size is not large enough for reporting

ANSI/AAMI CI86

The ANSI/AAMI CI86 Standard does not require reporting for devices older than 20 years after the last implantation of that device type. Please refer to the ISO data for information.

SOUND PROCESSOR STIMULATORS

For each currently-available sound processor, there will be a simple measure of reliability based on the average global yearly return rate and graphical data in compliance with ANSI/AAMI CI86 Standard that shows the monthly failure rate.

Where possible, this monthly data is further categorized into failure mechanisms, if known, to include mechanical, electronic, moisture damage, and other. Processors that meet all specifications are included and they are classified as no fault found. Where available, the number of registered users is shown, categorized into adult, children, and combined.




NAÍDA CI M AND SKY CI M

The Naída™ CI M sound processor for adults and Sky CI™ M sound processor for children are the newest Advanced Bionics products integrated with the latest advancements from Phonak, the Marvel platform. With built-in connectivity solutions and the ability to automatically sense and adapt to every situation, the Naída CI M and Sky CI M processors are designed to give you the best hearing experience.

Reliability of the Naída CI M and Sky CI M sound processors are combined at this time due to the limited number of devices in use. As field data becomes available globally, we will present the reliability metrics as separate products in future reports.

RELIABILITY: 99.20%^a

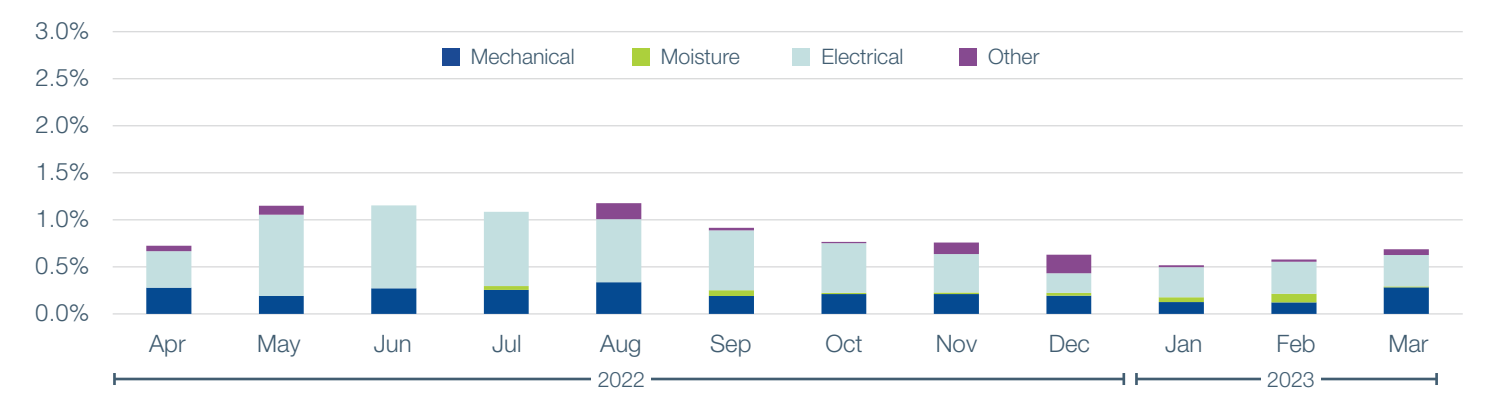

FAILED COMPONENT RETURN RATE^b

Cause	Apr 2022	May 2022	Jun 2022	Jul 2022	Aug 2022	Sep 2022	Oct 2022	Nov 2022	Dec 2022	Jan 2023	Feb 2023	Mar 2023
MECHANICAL	0.28%	0.19%	0.27%	0.26%	0.34%	0.19%	0.21%	0.21%	0.19%	0.13%	0.12%	0.28%
MOISTURE	0.00%	0.00%	0.00%	0.04%	0.00%	0.06%	0.02%	0.02%	0.03%	0.05%	0.09%	0.01%
ELECTRICAL	0.39%	0.86%	0.88%	0.79%	0.67%	0.64%	0.53%	0.41%	0.21%	0.32%	0.34%	0.33%
OTHER	0.06%	0.10%	0.00%	0.00%	0.17%	0.03%	0.02%	0.12%	0.19%	0.02%	0.02%	0.06%

a. Reliability is 1 minus the return rate. The return rate is the average global monthly return rate between April 2022 and March 2023.
b. The number per month represent the unit that complete failure analysis in that month.




NAÍDA CI Q SERIES

The Naída™ CI Q sound processors feature state-of-the-art technologies exclusively available from Advanced Bionics and Phonak for the best possible hearing experience.



RELIABILITY: 99.85%^a

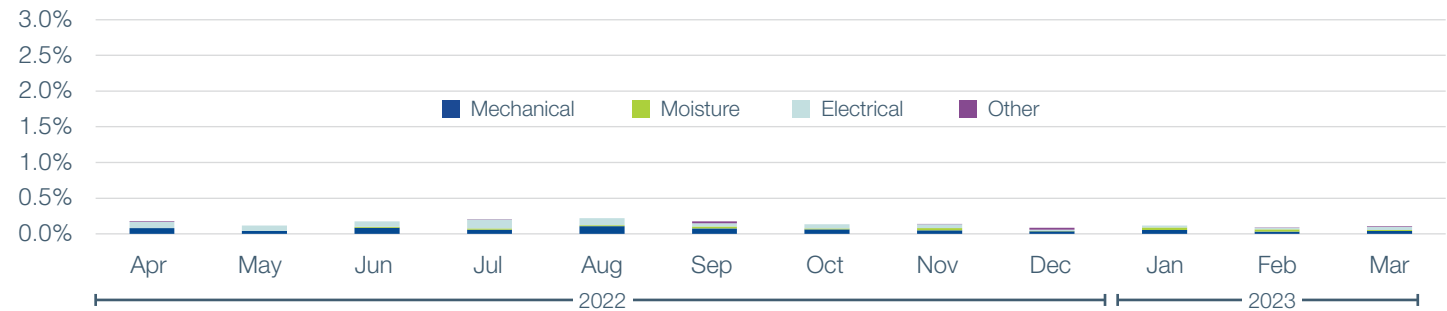

FAILED COMPONENT RETURN RATE^b


Cause	Apr 2022	May 2022	Jun 2022	Jul 2022	Aug 2022	Sep 2022	Oct 2022	Nov 2022	Dec 2022	Jan 2023	Feb 2023	Mar 2023
MECHANICAL	0.08%	0.04%	0.08%	0.06%	0.11%	0.08%	0.06%	0.05%	0.04%	0.05%	0.03%	0.04%
MOISTURE	0.00%	0.00%	0.01%	0.02%	0.01%	0.02%	0.02%	0.03%	0.00%	0.04%	0.03%	0.01%
ELECTRICAL	0.09%	0.08%	0.08%	0.12%	0.10%	0.05%	0.06%	0.06%	0.02%	0.03%	0.03%	0.04%
OTHER	0.01%	0.00%	0.00%	0.01%	0.00%	0.02%	0.00%	0.01%	0.03%	0.00%	0.00%	0.01%

CHORUS

The Chorus™ sound processor is compatible with C1.0 and C1.2 cochlear implants, and offers integrated Roger™ technology for connectivity and performance.



RELIABILITY: 99.77%^a

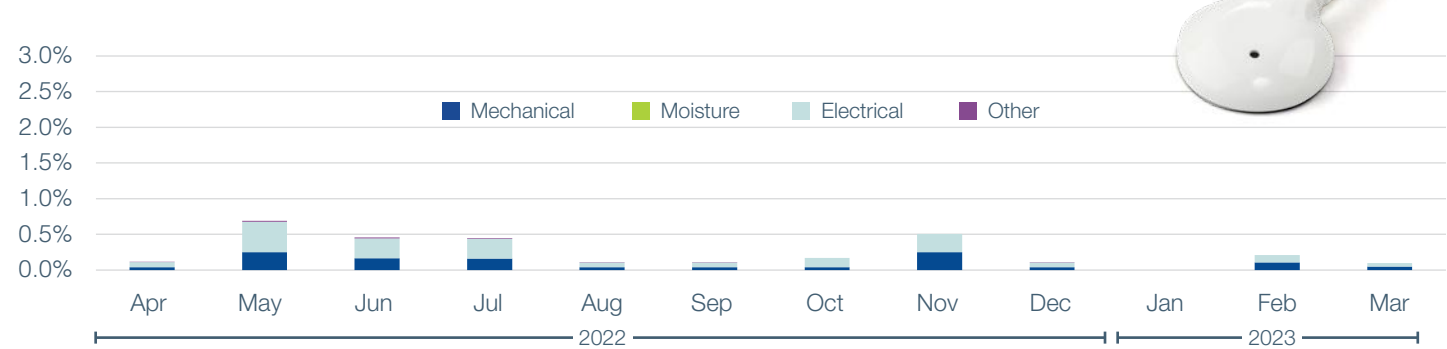

FAILED COMPONENT RETURN RATE^b


Cause	Apr 2022	May 2022	Jun 2022	Jul 2022	Aug 2022	Sep 2022	Oct 2022	Nov 2022	Dec 2022	Jan 2023	Feb 2023	Mar 2023
MECHANICAL	0.04%	0.25%	0.17%	0.16%	0.04%	0.04%	0.04%	0.25%	0.04%	0.00%	0.11%	0.05%
MOISTURE	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%
ELECTRICAL	0.07%	0.42%	0.28%	0.28%	0.07%	0.07%	0.13%	0.25%	0.07%	0.00%	0.11%	0.05%
OTHER	0.00%	0.02%	0.01%	0.01%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%

NEPTUNE

The Neptune™ sound processor is the first and only swimmable sound processor.



RELIABILITY: 99.95%^a

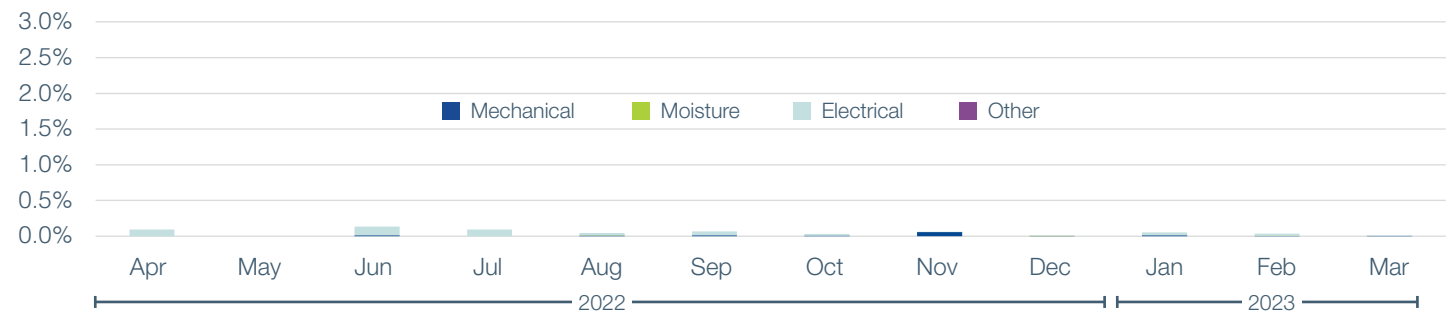

FAILED COMPONENT RETURN RATE^b

Cause	Apr 2022	May 2022	Jun 2022	Jul 2022	Aug 2022	Sep 2022	Oct 2022	Nov 2022	Dec 2022	Jan 2023	Feb 2023	Mar 2023
MECHANICAL	0.00%	0.00%	0.01%	0.00%	0.01%	0.01%	0.01%	0.06%	0.00%	0.01%	0.01%	0.00%
MOISTURE	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.01%	0.00%
ELECTRICAL	0.09%	0.00%	0.12%	0.09%	0.03%	0.05%	0.02%	0.01%	0.00%	0.04%	0.02%	0.01%
OTHER	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%	0.00%

a. Reliability is 1 minus the return rate. The return rate is the average global monthly return rate October 2021 to September 2022.

b. The number per month represent the unit that complete failure analysis in that month.

HIRES ULTRA 3D v2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.70%	0.01%	0.00%	0.71%	0.86%	0.57%
	1.5	0.84%	0.02%	0.00%	0.86%	1.03%	0.69%
	2	1.07%	0.02%	0.00%	1.09%	1.30%	0.88%
	2.5	1.17%	0.02%	0.00%	1.19%	1.44%	0.95%
	3	1.17%	0.02%	0.00%	1.19%	1.44%	0.95%
CHILDREN	1	0.58%	0.10%	0.00%	0.68%	0.95%	0.40%
	1.5	0.75%	0.10%	0.00%	0.85%	1.17%	0.53%
	2	0.75%	0.10%	0.00%	0.85%	1.17%	0.53%
	2.5	0.75%	0.10%	0.00%	0.85%	1.17%	0.53%
	3 ^a	N/A	N/A	N/A	N/A	N/A	N/A

HIRES ULTRA v2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.43%	0.00%	0.00%	0.43%	0.70%	0.16%
	1.5	0.50%	0.00%	0.00%	0.50%	0.79%	0.20%
	2	0.50%	0.00%	0.00%	0.50%	0.79%	0.20%
	2.5 ^a	N/A	N/A	N/A	N/A	N/A	N/A
CHILDREN	1	0.21%	0.03%	0.00%	0.25%	0.43%	0.06%
	1.5	0.21%	0.03%	0.00%	0.25%	0.43%	0.06%
	2	0.21%	0.03%	0.00%	0.25%	0.43%	0.06%
	2.5 ^a	N/A	N/A	N/A	N/A	N/A	N/A

HIRES ULTRA 3D v1

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.93%	0.13%	0.02%	1.09%	1.37%	0.81%
	1.5	1.37%	0.71%	0.10%	2.17%	2.57%	1.78%
	2	1.70%	2.40%	0.18%	4.24%	4.78%	3.69%
	2.5	2.08%	5.02%	0.20%	7.18%	7.88%	6.48%
	3	2.39%	8.14%	0.22%	10.54%	11.37%	9.70%
	3.5	2.62%	11.26%	0.27%	13.81%	14.77%	12.85%
	4	2.71%	13.66%	0.27%	16.23%	17.33%	15.12%
CHILDREN	1	1.11%	0.49%	0.00%	1.60%	2.25%	0.95%
	1.5	1.54%	2.19%	0.00%	3.69%	4.67%	2.72%
	2	1.98%	7.40%	0.15%	9.37%	10.88%	7.86%
	2.5	2.69%	12.92%	0.15%	15.39%	17.27%	13.52%
	3	3.89%	18.87%	0.15%	22.15%	24.32%	19.98%
	3.5	4.00%	22.21%	0.15%	25.44%	27.75%	23.12%
	4 ^a	N/A	N/A	N/A	N/A	N/A	N/A

HIRES ULTRA v1

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.77%	0.03%	0.02%	0.82%	1.02%	0.63%
	2	1.30%	0.45%	0.05%	1.79%	2.07%	1.51%
	3	1.75%	3.20%	0.11%	5.00%	5.46%	4.54%
	4	1.98%	8.91%	0.16%	10.86%	11.54%	10.19%
	5	2.12%	15.17%	0.16%	17.10%	17.99%	16.22%
	6	2.21%	19.97%	0.16%	21.87%	23.03%	20.71%
CHILDREN	1	0.56%	0.13%	0.00%	0.69%	0.95%	0.43%
	2	0.82%	1.28%	0.05%	2.14%	2.60%	1.69%
	3	1.08%	6.27%	0.11%	7.39%	8.21%	6.57%
	4	1.63%	15.72%	0.11%	17.18%	18.43%	15.93%
	5	1.82%	24.42%	0.17%	25.92%	27.58%	24.26%
	6 ^a	N/A	N/A	N/A	N/A	N/A	N/A

HIRES 90K ADVANTAGE

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
ADULTS	1	0.65%	0.06%	0.01%	0.73%	0.85%	0.61%
	2	1.12%	0.08%	0.02%	1.22%	1.37%	1.07%
	3	1.38%	0.13%	0.03%	1.54%	1.71%	1.37%
	4	1.66%	0.18%	0.03%	1.87%	2.06%	1.69%
	5	1.90%	0.20%	0.04%	2.14%	2.34%	1.94%
	6	2.02%	0.23%	0.05%	2.29%	2.50%	2.08%
	7	2.16%	0.24%	0.05%	2.45%	2.67%	2.23%
	8	2.28%	0.27%	0.05%	2.60%	2.84%	2.37%
	9	2.33%	0.31%	0.07%	2.71%	2.95%	2.46%
	10	2.46%	0.31%	0.12%	2.88%	3.17%	2.58%
CHILDREN	1	0.71%	0.19%	0.02%	0.93%	1.05%	0.80%
	2	1.02%	0.37%	0.04%	1.42%	1.58%	1.26%
	3	1.28%	0.56%	0.04%	1.87%	2.05%	1.68%
	4	1.51%	0.70%	0.08%	2.28%	2.49%	2.07%
	5	1.66%	0.87%	0.12%	2.63%	2.86%	2.40%
	6	1.83%	1.00%	0.12%	2.94%	3.19%	2.69%
	7	1.97%	1.16%	0.14%	3.24%	3.51%	2.97%
	8	2.09%	1.27%	0.16%	3.50%	3.79%	3.20%
	9	2.12%	1.44%	0.22%	3.75%	4.09%	3.41%
	10	2.20%	1.59%	0.22%	3.96%	4.38%	3.55%

HIRES 90K vendor A post-mod

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
ADULTS	1	0.78%	0.07%	0.01%	0.86%	0.95%	0.77%
	2	1.29%	0.11%	0.04%	1.44%	1.56%	1.32%
	3	1.59%	0.17%	0.06%	1.82%	1.95%	1.68%
	4	1.86%	0.24%	0.08%	2.18%	2.32%	2.03%
	5	2.10%	0.28%	0.09%	2.46%	2.61%	2.31%
	6	2.25%	0.34%	0.10%	2.68%	2.84%	2.52%
	7	2.39%	0.36%	0.11%	2.86%	3.02%	2.69%
	8	2.53%	0.43%	0.12%	3.07%	3.24%	2.89%
	9	2.63%	0.47%	0.13%	3.21%	3.39%	3.03%
	10	2.75%	0.53%	0.14%	3.40%	3.59%	3.21%
	11	2.85%	0.57%	0.14%	3.54%	3.74%	3.35%
	12	2.97%	0.59%	0.15%	3.68%	3.89%	3.47%
	13	3.10%	0.60%	0.16%	3.84%	4.06%	3.62%
	14	3.23%	0.62%	0.17%	4.00%	4.23%	3.77%
	15	3.36%	0.63%	0.17%	4.14%	4.38%	3.90%
	16	3.44%	0.70%	0.17%	4.28%	4.55%	4.02%
	17	3.49%	0.74%	0.17%	4.37%	4.67%	4.08%
CHILDREN	1	0.78%	0.19%	0.03%	1.00%	1.10%	0.91%
	2	1.10%	0.46%	0.04%	1.59%	1.71%	1.47%
	3	1.35%	0.72%	0.06%	2.12%	2.26%	1.98%
	4	1.55%	0.96%	0.08%	2.58%	2.73%	2.42%
	5	1.73%	1.18%	0.11%	3.00%	3.17%	2.84%
	6	1.87%	1.35%	0.12%	3.32%	3.50%	3.14%
	7	2.00%	1.49%	0.14%	3.59%	3.77%	3.40%
	8	2.08%	1.63%	0.16%	3.83%	4.02%	3.63%
	9	2.18%	1.73%	0.18%	4.05%	4.26%	3.84%
	10	2.37%	1.87%	0.22%	4.40%	4.63%	4.18%
	11	2.54%	1.89%	0.24%	4.61%	4.85%	4.37%
	12	2.71%	1.99%	0.29%	4.92%	5.18%	4.66%
	13	2.87%	2.01%	0.29%	5.10%	5.37%	4.82%
	14	2.99%	2.09%	0.31%	5.30%	5.60%	5.01%
	15	3.16%	2.17%	0.35%	5.60%	5.93%	5.26%
	16	3.30%	2.32%	0.42%	5.94%	6.34%	5.55%
	17	3.38%	2.40%	0.42%	6.10%	6.56%	5.65%

HIRES 90K vendor A all

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.77%	0.08%	0.01%	0.87%	0.96%	0.78%
	2	1.28%	0.14%	0.05%	1.47%	1.58%	1.35%
	3	1.58%	0.20%	0.08%	1.86%	1.99%	1.73%
	4	1.85%	0.31%	0.10%	2.25%	2.39%	2.11%
	5	2.08%	0.36%	0.11%	2.55%	2.70%	2.39%
	6	2.23%	0.44%	0.13%	2.78%	2.94%	2.62%
	7	2.38%	0.47%	0.14%	2.98%	3.15%	2.81%
	8	2.52%	0.57%	0.14%	3.21%	3.39%	3.04%
	9	2.61%	0.65%	0.15%	3.40%	3.58%	3.21%
	10	2.74%	0.73%	0.17%	3.61%	3.80%	3.42%
	11	2.84%	0.80%	0.17%	3.78%	3.98%	3.58%
	12	2.97%	0.86%	0.18%	3.97%	4.18%	3.76%
	13	3.09%	0.90%	0.20%	4.16%	4.38%	3.94%
	14	3.25%	0.98%	0.21%	4.39%	4.63%	4.16%
	15	3.37%	1.02%	0.21%	4.55%	4.80%	4.30%
	16	3.46%	1.10%	0.21%	4.72%	4.99%	4.45%
	17	3.54%	1.24%	0.23%	4.96%	5.27%	4.65%
	18	3.59%	1.34%	0.23%	5.11%	5.46%	4.76%
	19	3.59%	1.43%	0.23%	5.19%	5.58%	4.80%
CHILDREN	1	0.79%	0.21%	0.03%	1.02%	1.12%	0.93%
	2	1.11%	0.48%	0.04%	1.62%	1.74%	1.50%
	3	1.37%	0.75%	0.06%	2.17%	2.31%	2.03%
	4	1.57%	1.01%	0.09%	2.65%	2.80%	2.49%
	5	1.75%	1.24%	0.12%	3.09%	3.26%	2.92%
	6	1.89%	1.43%	0.13%	3.42%	3.60%	3.24%
	7	2.02%	1.59%	0.15%	3.72%	3.91%	3.53%
	8	2.12%	1.75%	0.17%	4.01%	4.21%	3.81%
	9	2.22%	1.87%	0.20%	4.23%	4.44%	4.02%
	10	2.41%	2.03%	0.24%	4.61%	4.84%	4.38%
	11	2.59%	2.07%	0.26%	4.86%	5.10%	4.62%
	12	2.74%	2.24%	0.31%	5.22%	5.48%	4.95%
	13	2.89%	2.29%	0.31%	5.41%	5.69%	5.13%
	14	3.00%	2.46%	0.33%	5.69%	5.99%	5.39%
	15	3.18%	2.61%	0.36%	6.05%	6.39%	5.71%
	16	3.29%	2.86%	0.42%	6.45%	6.85%	6.06%
	17	3.34%	3.01%	0.42%	6.65%	7.09%	6.21%
	18	3.53%	3.20%	0.42%	7.02%	7.58%	6.45%
	19	3.90%	3.20%	0.42%	7.37%	8.11%	6.62%

HIRES 90K vendor A pre-mod

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	
						CI Higher	CI Lower
ADULTS	1	0.60%	0.42%	0.00%	1.02%	1.51%	0.54%
	2	1.03%	0.85%	0.24%	2.11%	2.80%	1.42%
	3	1.33%	1.09%	0.49%	2.89%	3.70%	2.09%
	4	1.58%	1.89%	0.55%	3.98%	4.92%	3.04%
	5	1.70%	2.32%	0.62%	4.58%	5.59%	3.57%
	6	1.83%	2.76%	0.68%	5.18%	6.25%	4.12%
	7	2.14%	3.00%	0.74%	5.79%	6.91%	4.66%
	8	2.20%	3.56%	0.74%	6.39%	7.57%	5.21%
	9	2.27%	4.25%	0.74%	7.11%	8.35%	5.88%
	10	2.39%	4.62%	0.81%	7.66%	8.94%	6.38%
	11	2.52%	5.00%	0.81%	8.14%	9.46%	6.82%
	12	2.78%	5.44%	0.81%	8.81%	10.17%	7.44%
	13	2.84%	5.69%	0.87%	9.17%	10.56%	7.78%
	14	3.17%	6.13%	0.87%	9.90%	11.33%	8.46%
	15	3.23%	6.32%	0.87%	10.14%	11.59%	8.68%
	16	3.37%	6.44%	0.87%	10.38%	11.85%	8.91%
	17	3.50%	6.70%	0.94%	10.81%	12.30%	9.31%
	18	3.56%	6.83%	0.94%	10.99%	12.50%	9.48%
	19	3.56%	6.91%	0.94%	11.07%	12.59%	9.56%

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
CHILDREN	1	1.25%	0.80%	0.00%	2.03%	2.96%	1.10%
	2	1.48%	1.37%	0.12%	2.94%	4.05%	1.83%
	3	2.06%	2.18%	0.23%	4.41%	5.77%	3.06%
	4	2.41%	3.11%	0.23%	5.66%	7.19%	4.14%
	5	2.52%	3.93%	0.36%	6.69%	8.34%	5.04%
	6	2.64%	4.75%	0.48%	7.71%	9.47%	5.95%
	7	3.13%	5.57%	0.72%	9.19%	11.10%	7.28%
	8	3.74%	6.52%	0.72%	10.67%	12.70%	8.63%
	9	3.74%	6.88%	0.72%	11.01%	13.07%	8.94%
	10	3.86%	7.48%	0.85%	11.80%	13.93%	9.67%
	11	4.23%	7.84%	0.98%	12.60%	14.79%	10.41%
	12	4.23%	8.80%	0.98%	13.51%	15.77%	11.26%
	13	4.23%	9.16%	0.98%	13.86%	16.14%	11.57%
	14	4.23%	10.00%	0.98%	14.66%	16.99%	12.32%
	15	4.49%	10.49%	0.98%	15.34%	17.72%	12.96%
	16	4.49%	11.09%	0.98%	15.91%	18.33%	13.50%
	17	4.49%	11.33%	0.98%	16.14%	18.57%	13.71%
	18	4.62%	11.58%	0.98%	16.49%	18.95%	14.04%
	19	5.01%	11.58%	0.98%	16.83%	19.32%	14.34%

HIRES 90K vendor B

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
ADULTS	1	0.95%	3.03%	0.00%	3.95%	4.71%	3.20%
	2	1.33%	10.84%	0.09%	12.10%	13.37%	10.84%
	3	1.56%	16.18%	0.18%	17.63%	19.11%	16.16%
	4	1.85%	20.72%	0.18%	22.32%	23.94%	20.70%
	5	1.95%	24.35%	0.23%	25.99%	27.70%	24.29%
	6	2.06%	26.69%	0.23%	28.37%	30.12%	26.61%
	7	2.17%	29.65%	0.23%	31.33%	33.14%	29.53%
	8	2.45%	31.52%	0.23%	33.35%	35.19%	31.52%
	9	2.45%	33.11%	0.23%	34.90%	36.75%	33.05%
	10	2.64%	34.54%	0.23%	36.41%	38.28%	34.54%
	11	2.64%	35.44%	0.23%	37.28%	39.17%	35.40%
	12	2.70%	36.75%	0.23%	38.60%	40.49%	36.70%
	13	2.76%	37.78%	0.23%	39.64%	41.54%	37.73%
	14	2.89%	38.56%	0.23%	40.47%	42.39%	38.56%
	15	2.96%	39.22%	0.23%	41.15%	43.07%	39.24%
	16	3.02%	39.68%	0.23%	41.63%	43.55%	39.71%
	17	3.09%	40.31%	0.23%	42.29%	44.21%	40.36%
	18	3.09%	40.80%	0.23%	42.76%	44.70%	40.82%
	19 ^a	N/A	N/A	N/A	N/A	N/A	N/A
CHILDREN	1	0.88%	3.28%	0.00%	4.13%	5.14%	3.13%
	2	1.31%	11.53%	0.07%	12.76%	14.45%	11.07%
	3	1.55%	19.82%	0.07%	21.13%	23.20%	19.06%
	4	1.55%	25.84%	0.07%	27.05%	29.30%	24.79%
	5	1.93%	30.51%	0.17%	31.97%	34.34%	29.60%
	6	2.13%	34.44%	0.17%	35.95%	38.39%	33.51%
	7	2.13%	37.69%	0.17%	39.12%	41.60%	36.64%
	8	2.35%	40.32%	0.17%	41.82%	44.33%	39.32%
	9	2.47%	42.68%	0.17%	44.19%	46.72%	41.67%
	10	2.47%	44.35%	0.17%	45.82%	48.35%	43.28%
	11	2.71%	45.47%	0.17%	47.04%	49.57%	44.50%
	12	3.09%	46.30%	0.43%	48.19%	50.73%	45.65%
	13	3.09%	47.85%	0.43%	49.68%	52.22%	47.13%
	14	3.22%	48.41%	0.56%	50.36%	52.90%	47.81%
	15	3.22%	49.33%	0.56%	51.24%	53.78%	48.70%
	16	3.22%	49.61%	0.70%	51.58%	54.12%	49.04%
	17	3.50%	50.34%	0.70%	52.42%	54.96%	49.87%
	18	3.71%	51.09%	0.70%	53.24%	55.80%	50.68%
	19 ^a	N/A	N/A	N/A	N/A	N/A	N/A

CII BIONIC EAR

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total	CI Higher	CI Lower
ADULTS	1	0.38%	0.38%	0.03%	0.80%		1.09%	0.50%
	2	0.65%	0.41%	0.18%	1.24%		1.61%	0.87%
	3	0.89%	0.59%	0.30%	1.77%		2.21%	1.33%
	4	1.19%	0.65%	0.39%	2.21%		2.71%	1.72%
	5	1.37%	0.74%	0.42%	2.51%		3.03%	1.98%
	6	1.46%	0.89%	0.48%	2.80%		3.36%	2.25%
	7	1.58%	0.95%	0.66%	3.16%		3.75%	2.57%
	8	1.70%	1.04%	0.75%	3.45%		4.07%	2.84%
	9	1.91%	1.14%	0.81%	3.81%		4.45%	3.17%
	10	2.03%	1.20%	0.81%	3.99%		4.65%	3.33%
	11	2.12%	1.29%	0.84%	4.20%		4.87%	3.52%
	12	2.33%	1.29%	0.87%	4.43%		5.13%	3.74%
	13	2.39%	1.29%	0.87%	4.49%		5.19%	3.79%
	14	2.45%	1.38%	0.87%	4.64%		5.35%	3.93%
	15	2.54%	1.44%	0.87%	4.79%		5.51%	4.07%
	16	2.60%	1.50%	0.87%	4.91%		5.64%	4.18%
	17	2.67%	1.56%	0.87%	5.03%		5.76%	4.29%
	18	2.76%	1.60%	0.94%	5.20%		5.95%	4.46%
	19	2.91%	1.66%	0.94%	5.42%		6.18%	4.65%
	20	3.11%	1.66%	0.94%	5.61%		6.39%	4.83%
	21	3.16%	1.70%	0.98%	5.75%		6.54%	4.96%
CHILDREN	1	0.23%	0.76%	0.06%	1.05%		1.53%	0.57%
	2	0.71%	1.41%	0.24%	2.33%		3.05%	1.62%
	3	1.30%	2.29%	0.30%	3.85%		4.77%	2.94%
	4	1.30%	2.77%	0.42%	4.44%		5.41%	3.46%
	5	1.61%	3.25%	0.72%	5.49%		6.57%	4.41%
	6	1.85%	4.03%	1.03%	6.78%		7.97%	5.59%
	7	1.98%	4.57%	1.16%	7.55%		8.80%	6.29%
	8	2.10%	5.00%	1.47%	8.37%		9.68%	7.05%
	9	2.29%	5.43%	1.60%	9.07%		10.43%	7.71%
	10	2.48%	5.79%	1.60%	9.60%		11.00%	8.20%
	11	2.61%	5.91%	1.79%	10.01%		11.43%	8.59%
	12	2.93%	6.04%	1.86%	10.48%		11.93%	9.03%
	13	3.24%	6.16%	1.92%	10.95%		12.43%	9.47%
	14	3.37%	6.41%	1.99%	11.36%		12.87%	9.86%
	15	3.44%	6.47%	1.99%	11.48%		12.99%	9.97%
	16	3.63%	6.53%	2.05%	11.77%		13.30%	10.25%
	17	3.89%	6.60%	2.18%	12.19%		13.74%	10.63%
	18	3.95%	6.72%	2.25%	12.42%		13.99%	10.86%
	19	4.56%	6.92%	2.25%	13.16%		14.76%	11.55%
	20	4.87%	6.92%	2.33%	13.51%		15.14%	11.88%
	21	5.20%	6.92%	2.33%	13.81%		15.47%	12.15%

CLARION 1.2

	Year	Medical CRP	Device CRP	Inconclusive CRP	Total All Categories	Total CI Higher	CI Lower
ADULTS	1	0.28%	0.28%	0.14%	0.71%	0.94%	0.47%
	2	0.39%	0.59%	0.22%	1.19%	1.49%	0.89%
	3	0.57%	1.26%	0.33%	2.14%	2.55%	1.74%
	4	0.78%	2.31%	0.49%	3.54%	4.06%	3.03%
	5	0.92%	3.59%	0.64%	5.09%	5.70%	4.48%
	6	1.10%	4.60%	0.73%	6.33%	7.01%	5.65%
	7	1.16%	5.47%	0.81%	7.32%	8.05%	6.60%
	8	1.36%	6.63%	0.94%	8.77%	9.56%	7.98%
	9	1.51%	7.32%	1.08%	9.71%	10.53%	8.88%
	10	1.76%	8.25%	1.28%	11.01%	11.89%	10.14%
	11	1.92%	8.98%	1.37%	11.95%	12.86%	11.05%
	12	2.21%	9.47%	1.58%	12.87%	13.81%	11.94%
	13	2.40%	9.92%	1.62%	13.51%	14.46%	12.55%
	14	2.58%	10.30%	1.72%	14.12%	15.09%	13.15%
	15	2.86%	10.73%	1.79%	14.84%	15.83%	13.84%
	16	3.21%	11.10%	1.86%	15.55%	16.57%	14.54%
	17	3.62%	11.55%	1.93%	16.40%	17.43%	15.36%
	18	4.33%	11.90%	1.93%	17.34%	18.40%	16.28%
	19	4.81%	12.23%	2.03%	18.15%	19.23%	17.07%
	20	5.39%	12.43%	2.10%	18.90%	19.99%	17.80%
	21	5.93%	12.62%	2.16%	19.58%	20.69%	18.46%
	22	6.24%	12.83%	2.26%	20.13%	21.25%	19.00%
	23	7.04%	13.12%	2.26%	21.06%	22.22%	19.91%
	24	7.62%	13.37%	2.36%	21.86%	23.05%	20.67%
	25	7.90%	13.44%	2.51%	22.28%	23.50%	21.05%
	26	8.29%	13.68%	2.51%	22.82%	24.12%	21.51%
CHILDREN	1	0.23%	1.68%	0.11%	2.02%	2.49%	1.56%
	2	0.38%	3.09%	0.20%	3.65%	4.27%	3.03%
	3	0.53%	5.26%	0.41%	6.14%	6.94%	5.35%
	4	0.77%	7.64%	0.54%	8.85%	9.79%	7.91%
	5	0.96%	9.96%	0.92%	11.64%	12.71%	10.58%
	6	1.26%	12.41%	1.22%	14.56%	15.73%	13.39%
	7	1.63%	14.31%	1.49%	16.96%	18.21%	15.72%
	8	1.91%	16.44%	1.84%	19.55%	20.87%	18.23%
	9	2.23%	17.78%	2.27%	21.44%	22.80%	20.07%
	10	2.49%	19.37%	2.81%	23.59%	25.00%	22.18%
	11	2.75%	20.48%	3.19%	25.14%	26.58%	23.69%
	12	2.98%	21.19%	3.45%	26.19%	27.65%	24.72%
	13	3.25%	21.85%	3.69%	27.18%	28.66%	25.70%
	14	3.57%	22.48%	3.80%	28.09%	29.59%	26.59%
	15	4.08%	23.62%	4.04%	29.70%	31.23%	28.18%
	16	4.85%	24.46%	4.36%	31.26%	32.81%	29.71%
	17	5.42%	25.08%	4.78%	32.53%	34.09%	30.96%
	18	6.51%	25.71%	4.99%	34.00%	35.59%	32.42%
	19	7.73%	26.21%	5.16%	35.43%	37.03%	33.83%
	20	9.07%	26.59%	5.34%	36.81%	38.43%	35.20%
	21	9.98%	26.96%	5.53%	37.89%	39.52%	36.26%
	22	11.23%	27.61%	5.79%	39.46%	41.11%	37.81%
	23	12.01%	28.20%	5.92%	40.56%	42.23%	38.89%
	24	13.06%	28.56%	6.11%	41.68%	43.39%	39.97%
	25	13.77%	29.02%	6.11%	42.54%	44.31%	40.76%
	26	14.81%	29.24%	6.68%	43.75%	45.70%	41.80%

CONTACT US

This report is intended to provide both professionals and our CI recipients with relevant information on the reliability of our products. If you have any questions, please contact us by emailing hear@AdvancedBionics.com or visit AdvancedBionics.com for more general information.



ADVANCED BIONICS LLC

28515 Westinghouse Place
Valencia, CA 91355, United States

T: +1.877.829.0026

T: +1.661.362.1400

F: +1.661.362.1500

info.us@advancedbionics.com

ADVANCED BIONICS AG

Laubisrütistrasse 28
8712 Stäfa, Switzerland

T: +41.58.928.78.00

F: +41.58.928.78.90

info.switzerland@advancedbionics.com

For information on additional AB locations, please visit advancedbionics.com/contact

Advanced Bionics – A Sonova brand

Please contact your local AB representative for regulatory approval and availability in your region.